





1/26

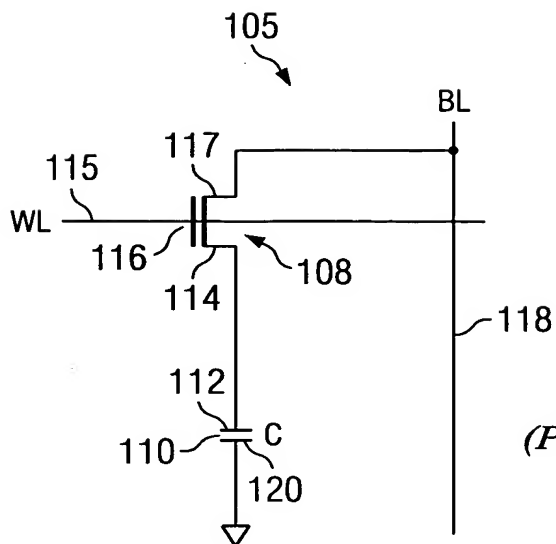



**FIG. 1**  
(PRIOR ART)

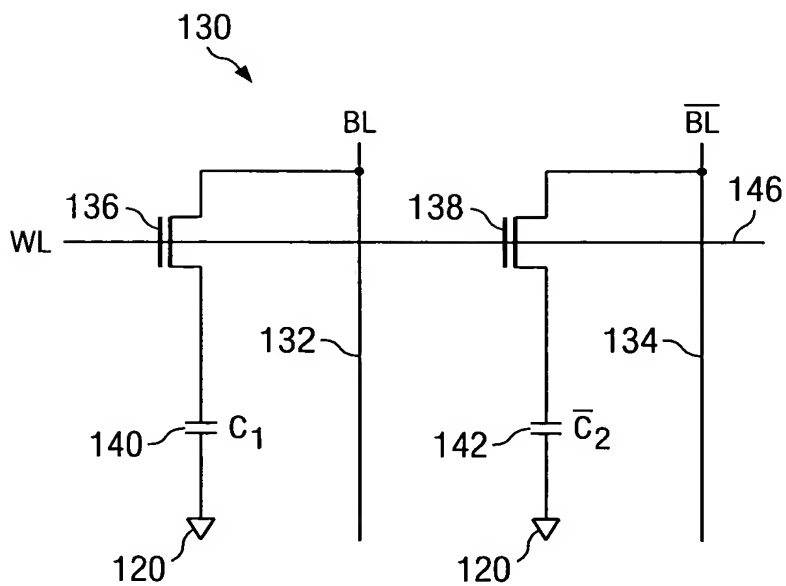

**FIG. 2**  
(PRIOR ART)

2/26

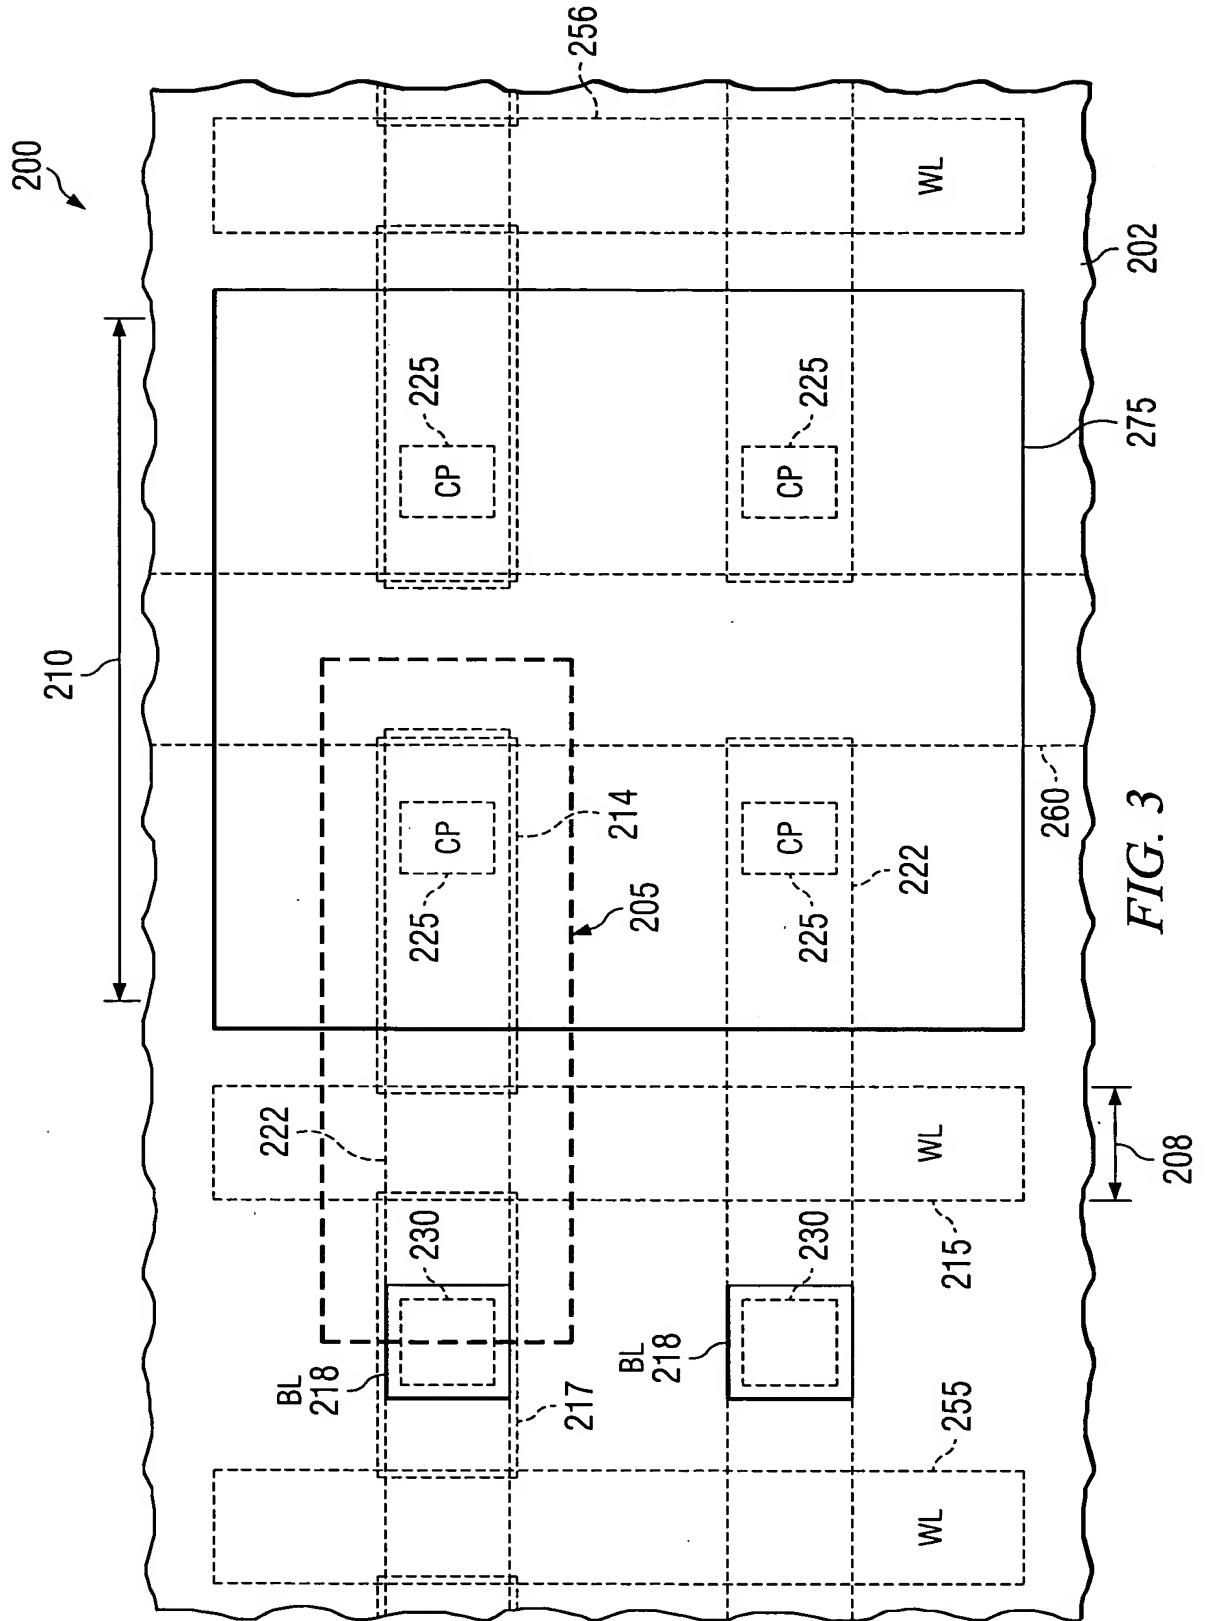

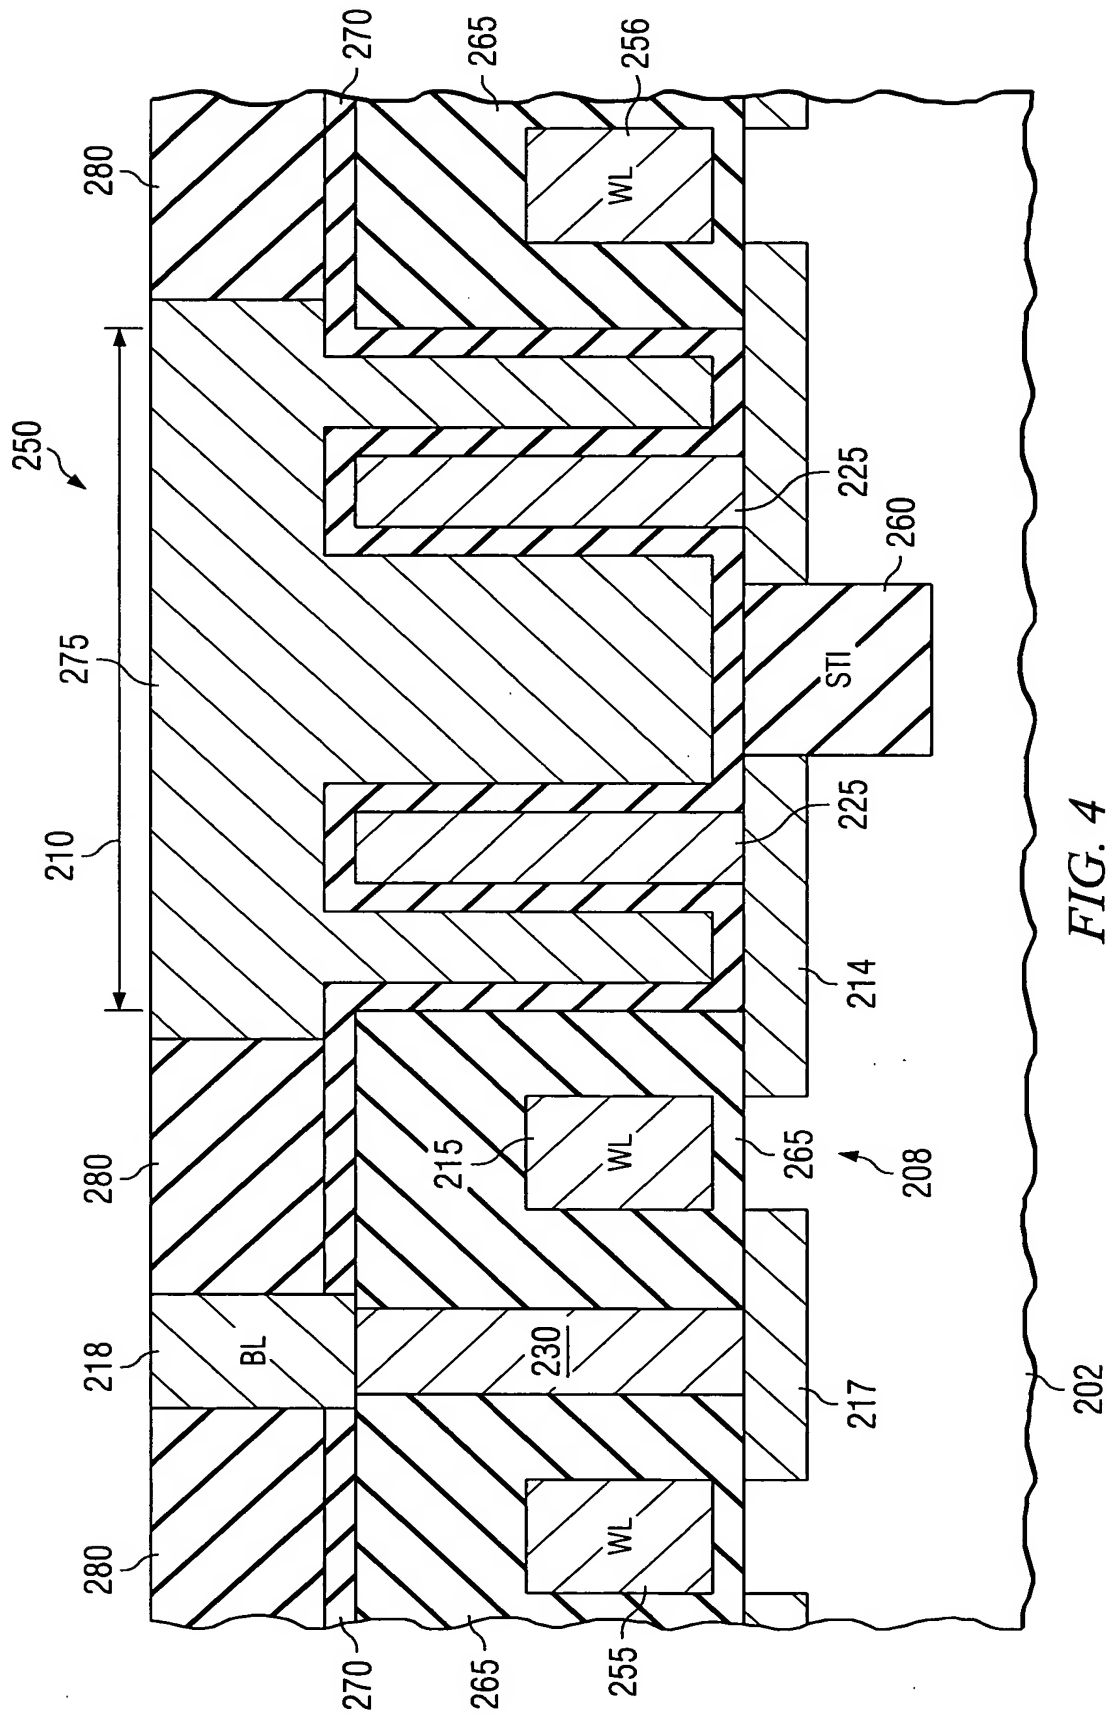

**FIG. 4**

4/26

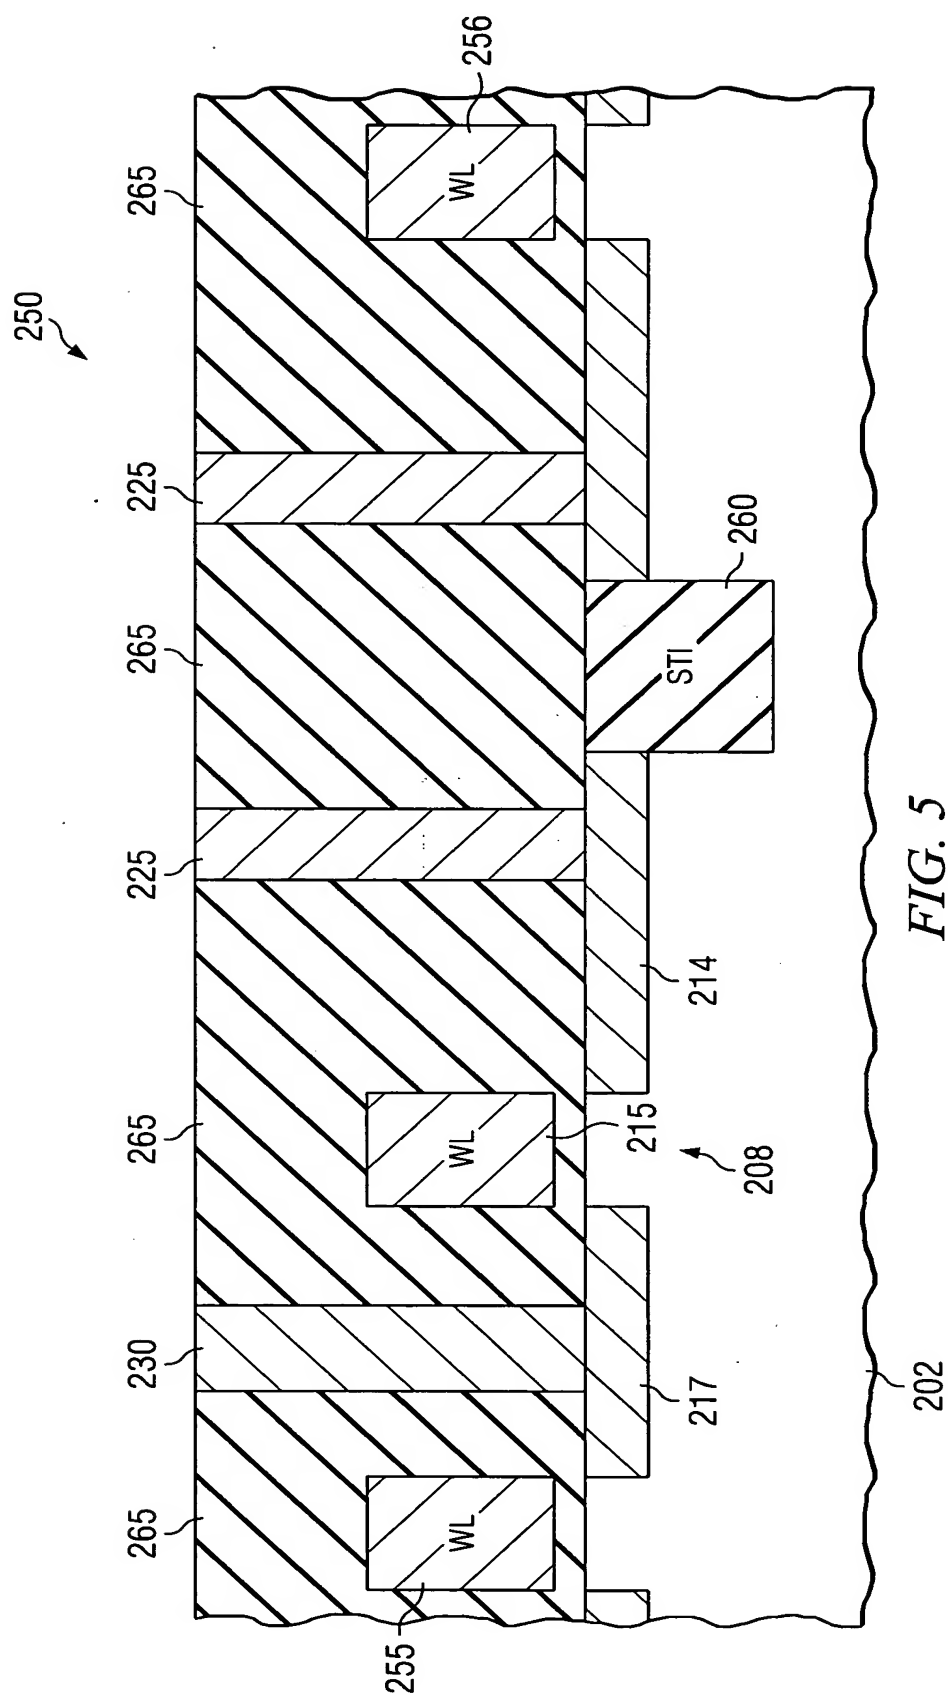


FIG. 5

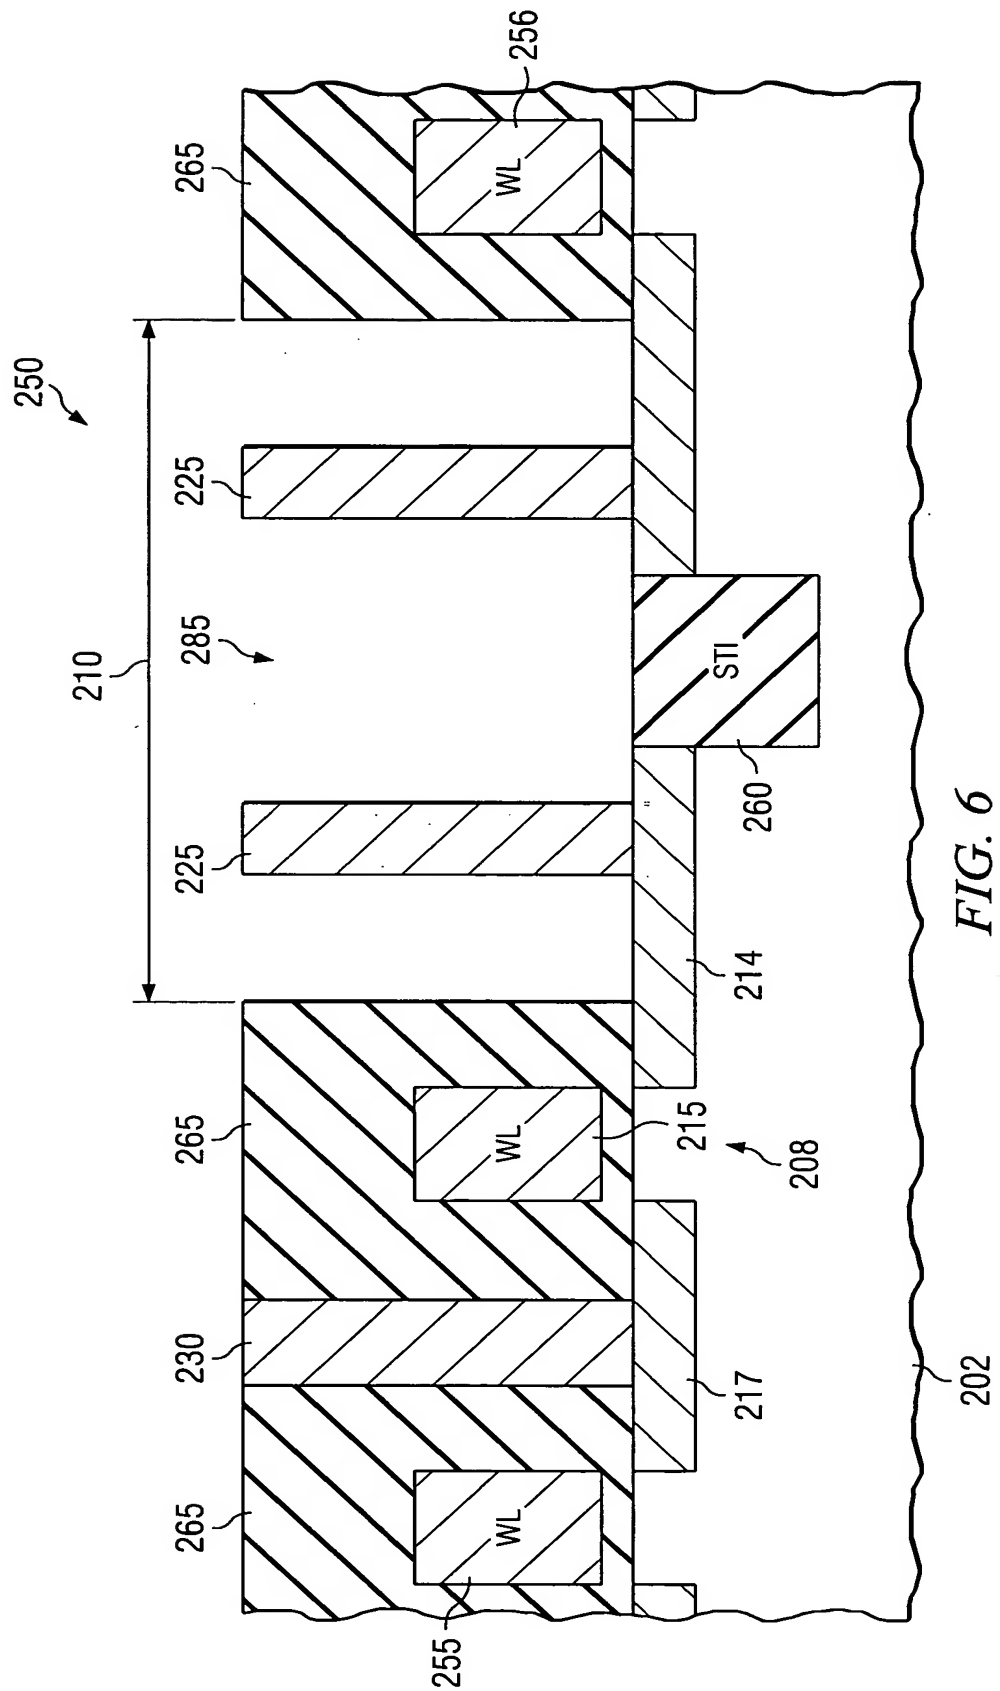


FIG. 6



7/26

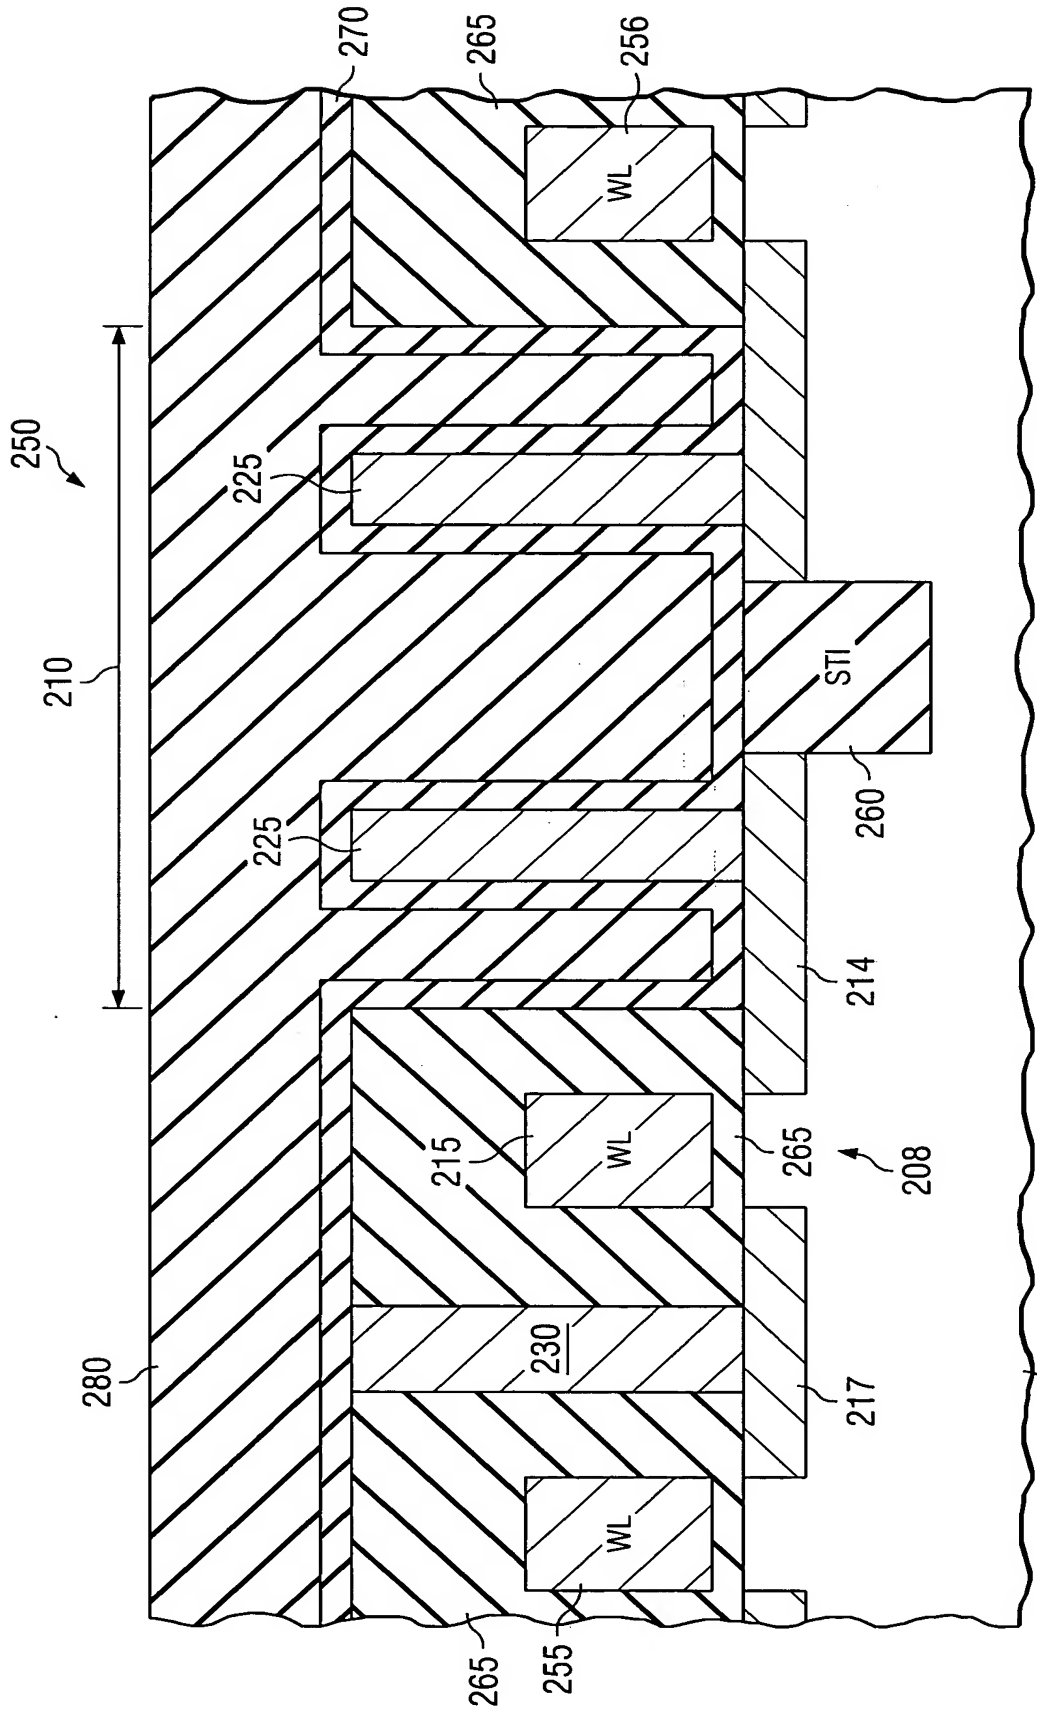


FIG. 8

8/26

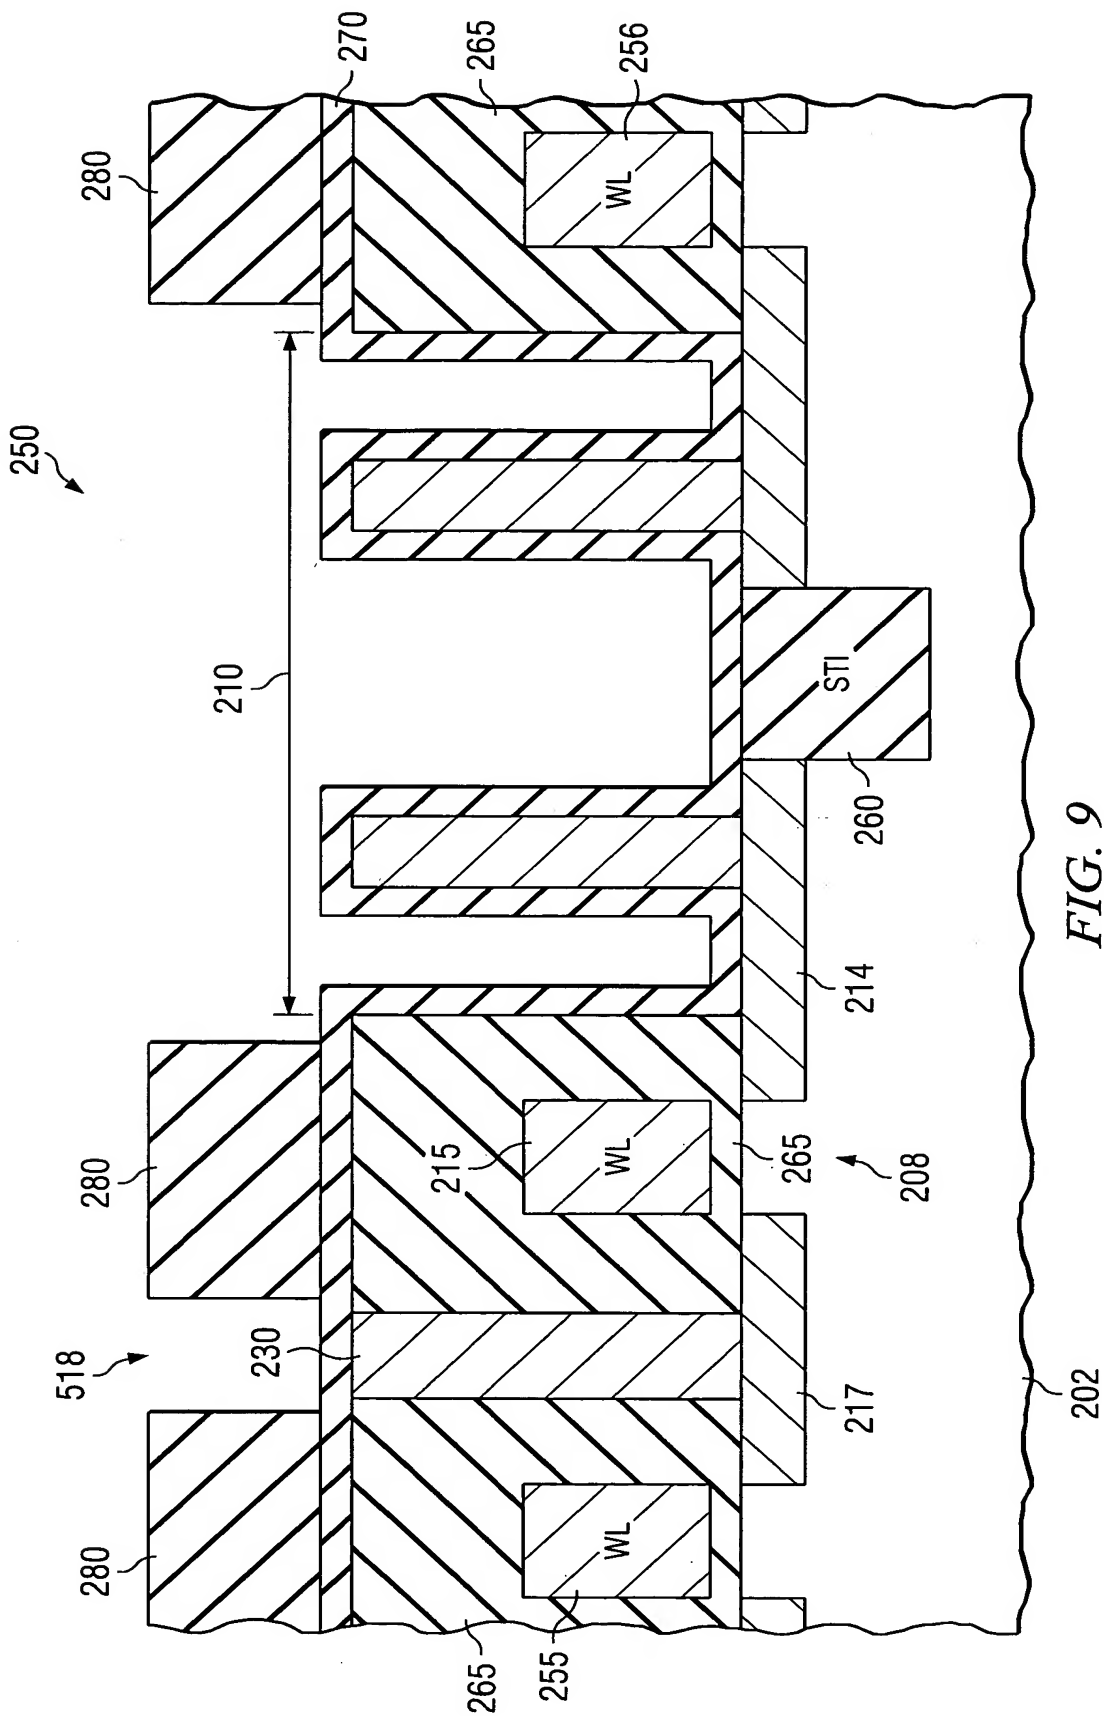


FIG. 9



9/26



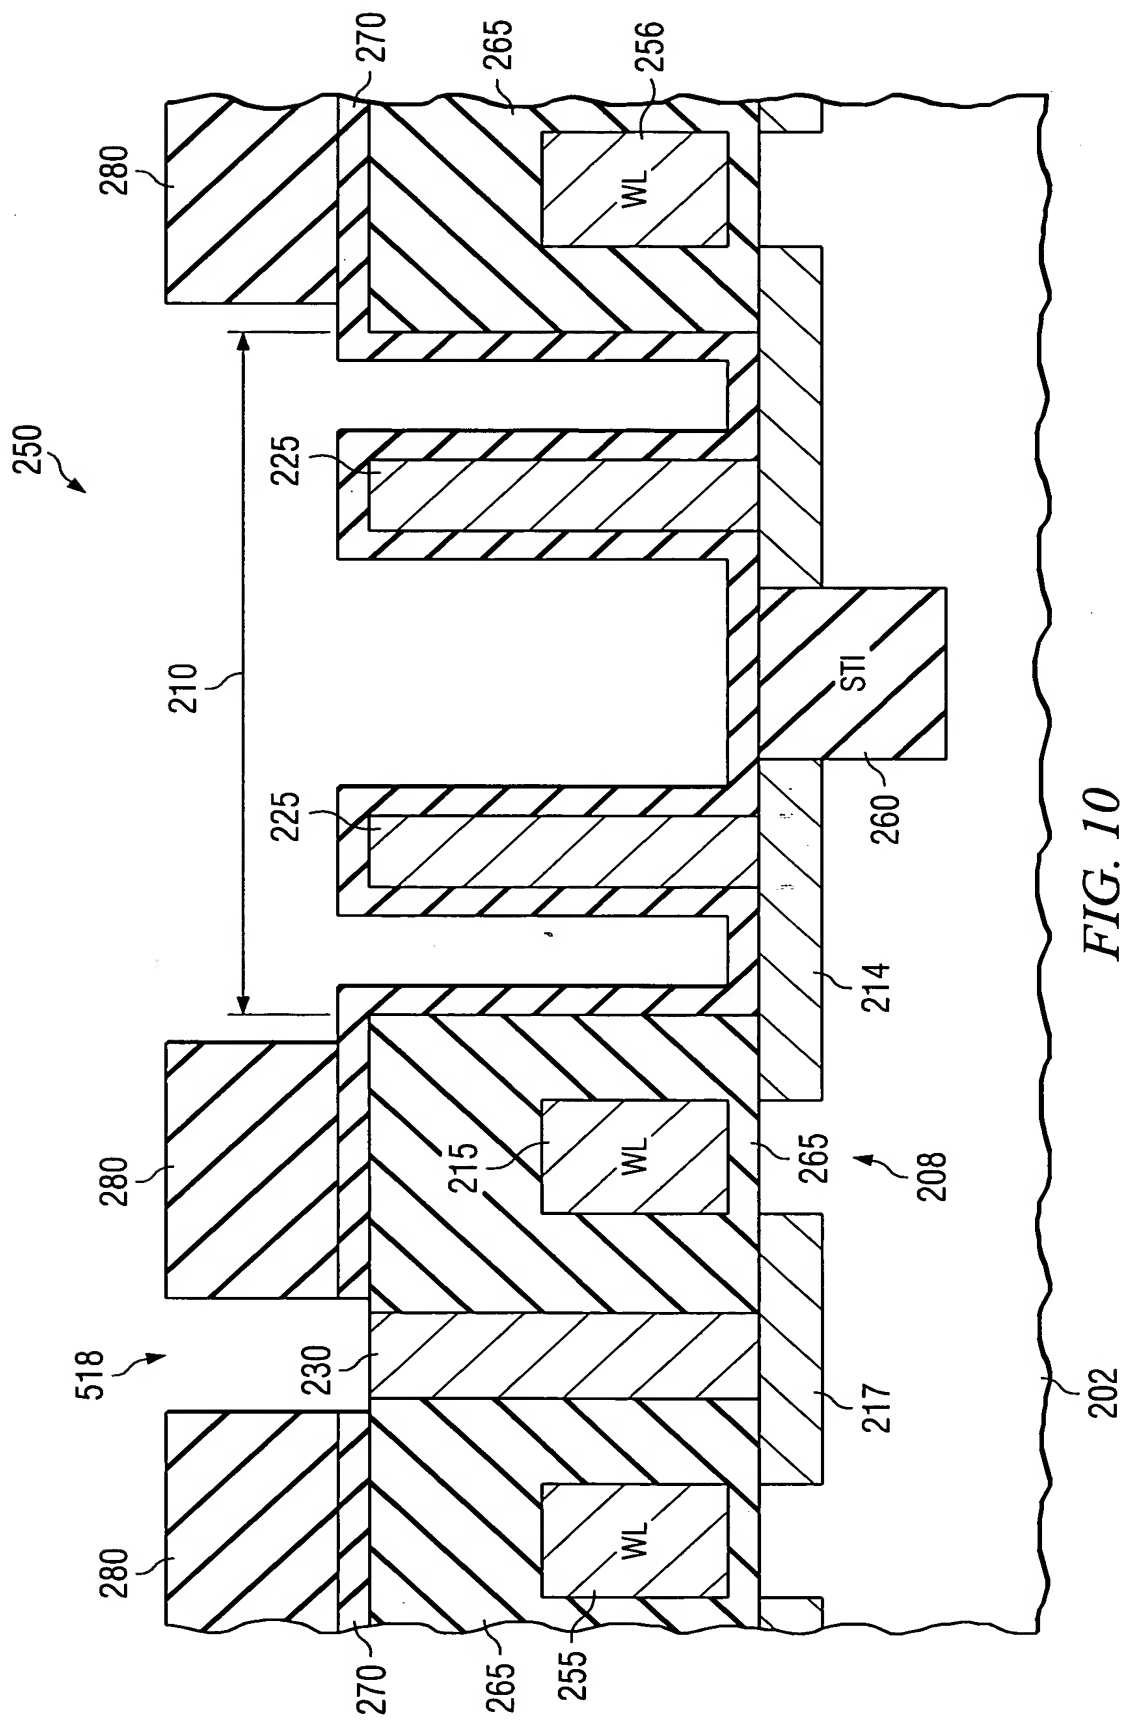


FIG. 10

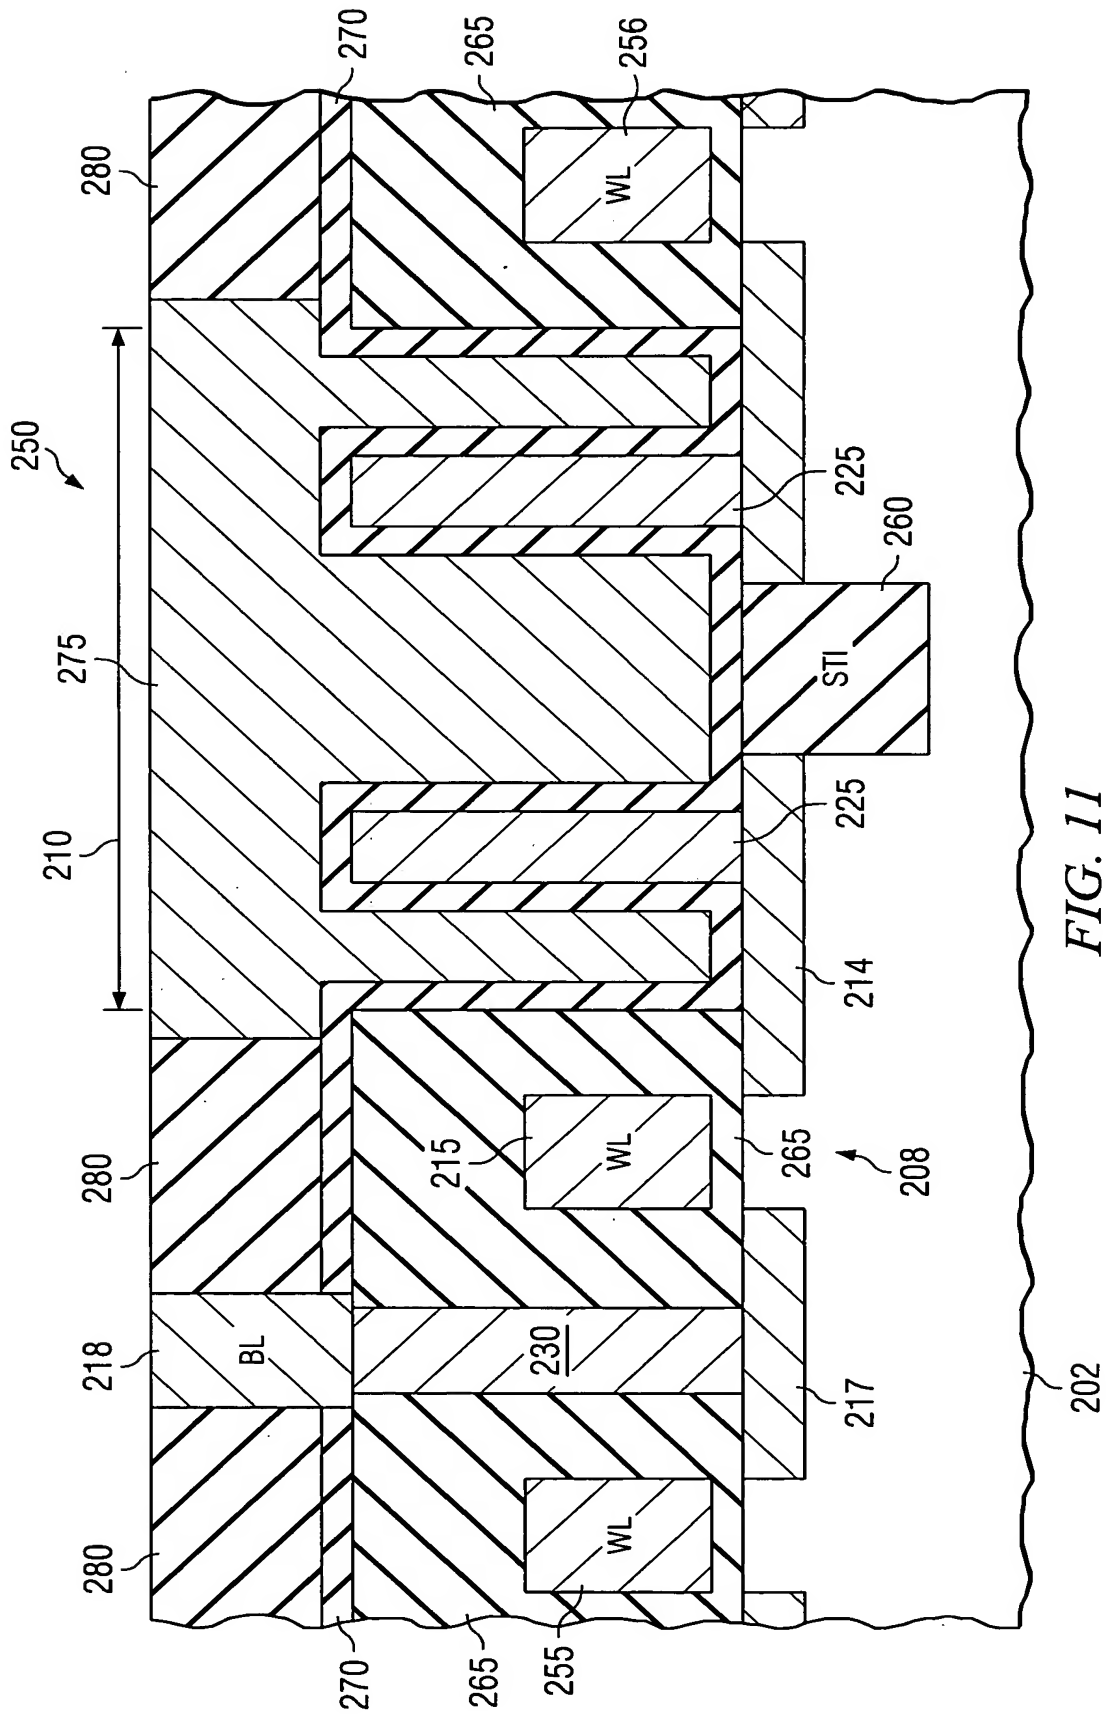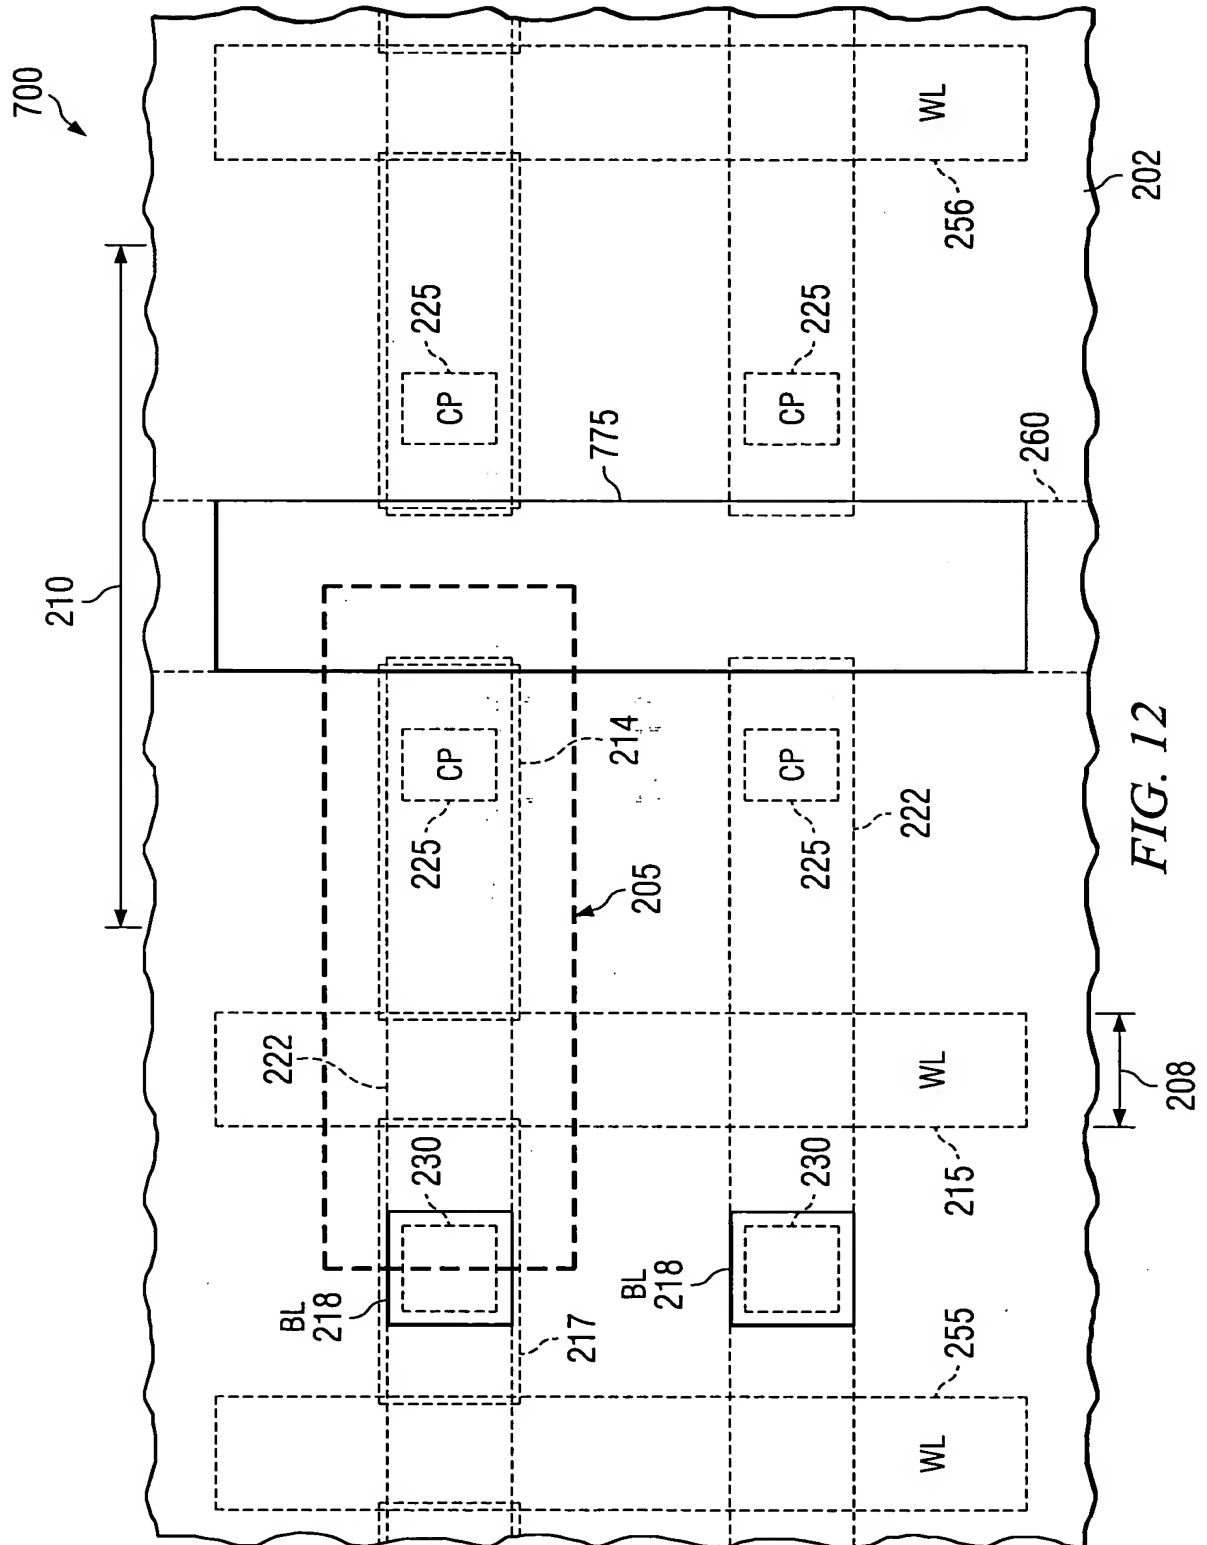

202



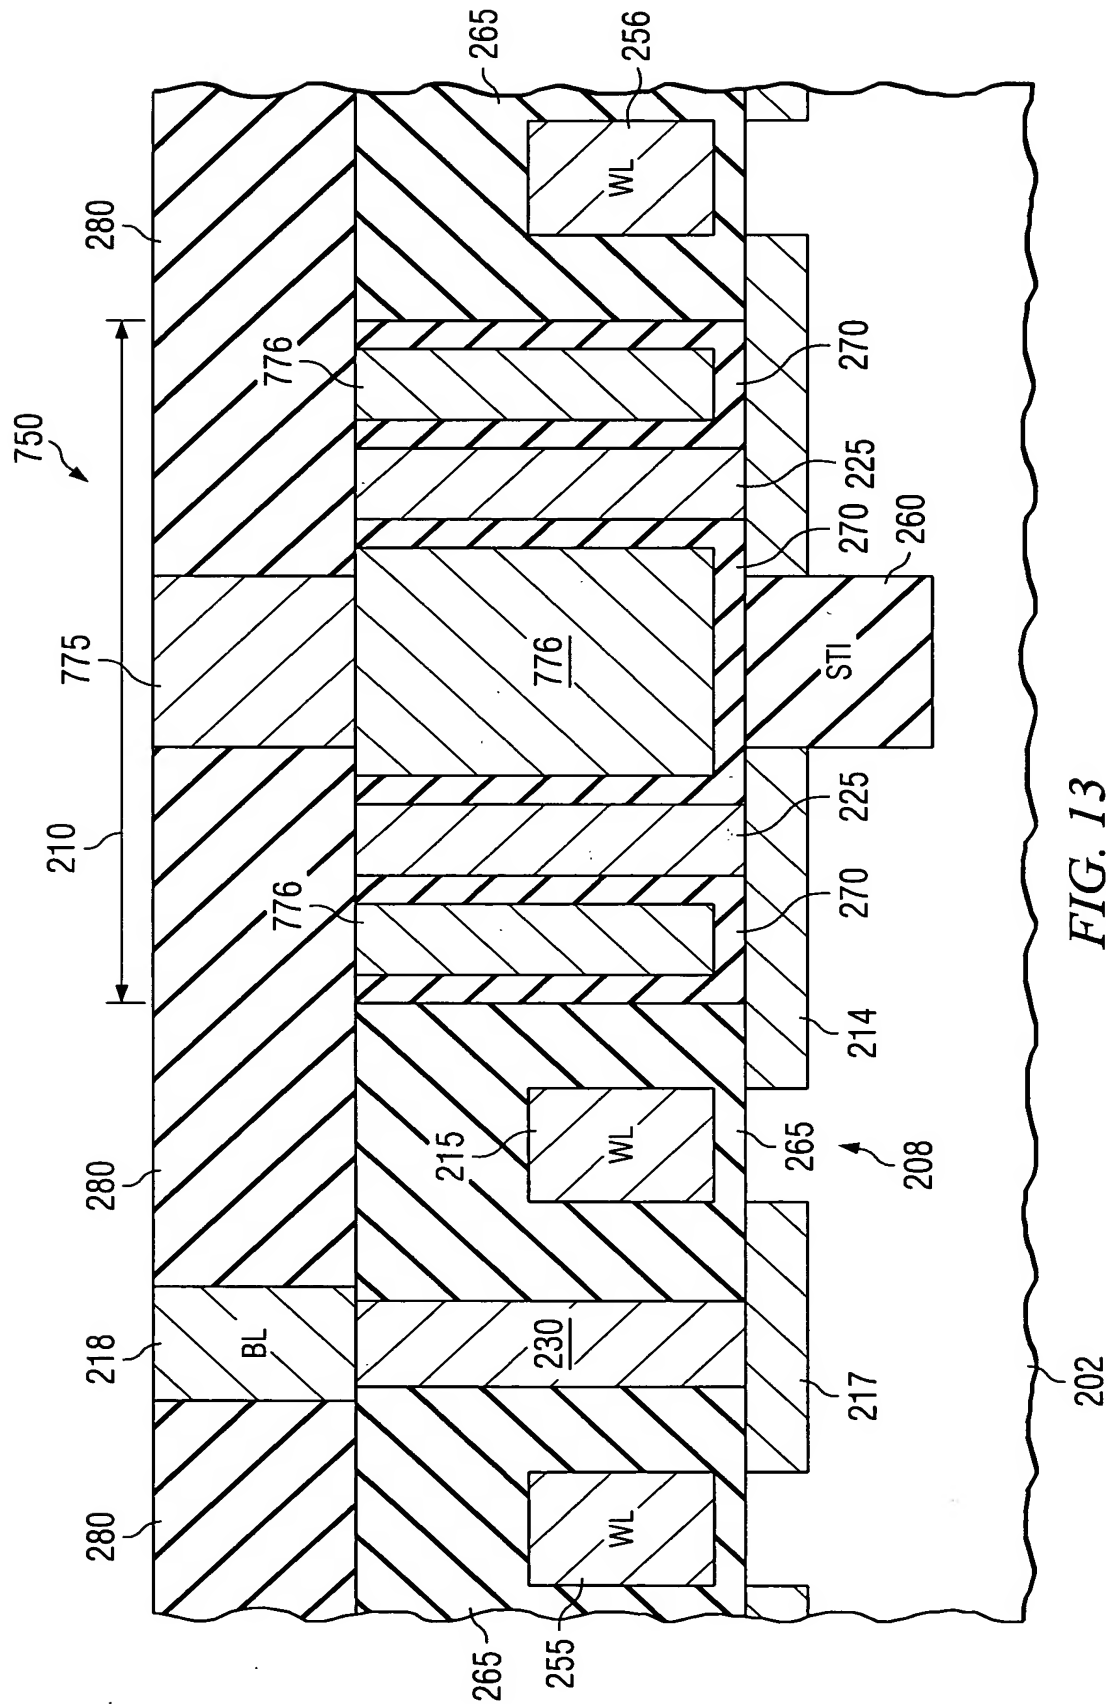


FIG. 13





15/26




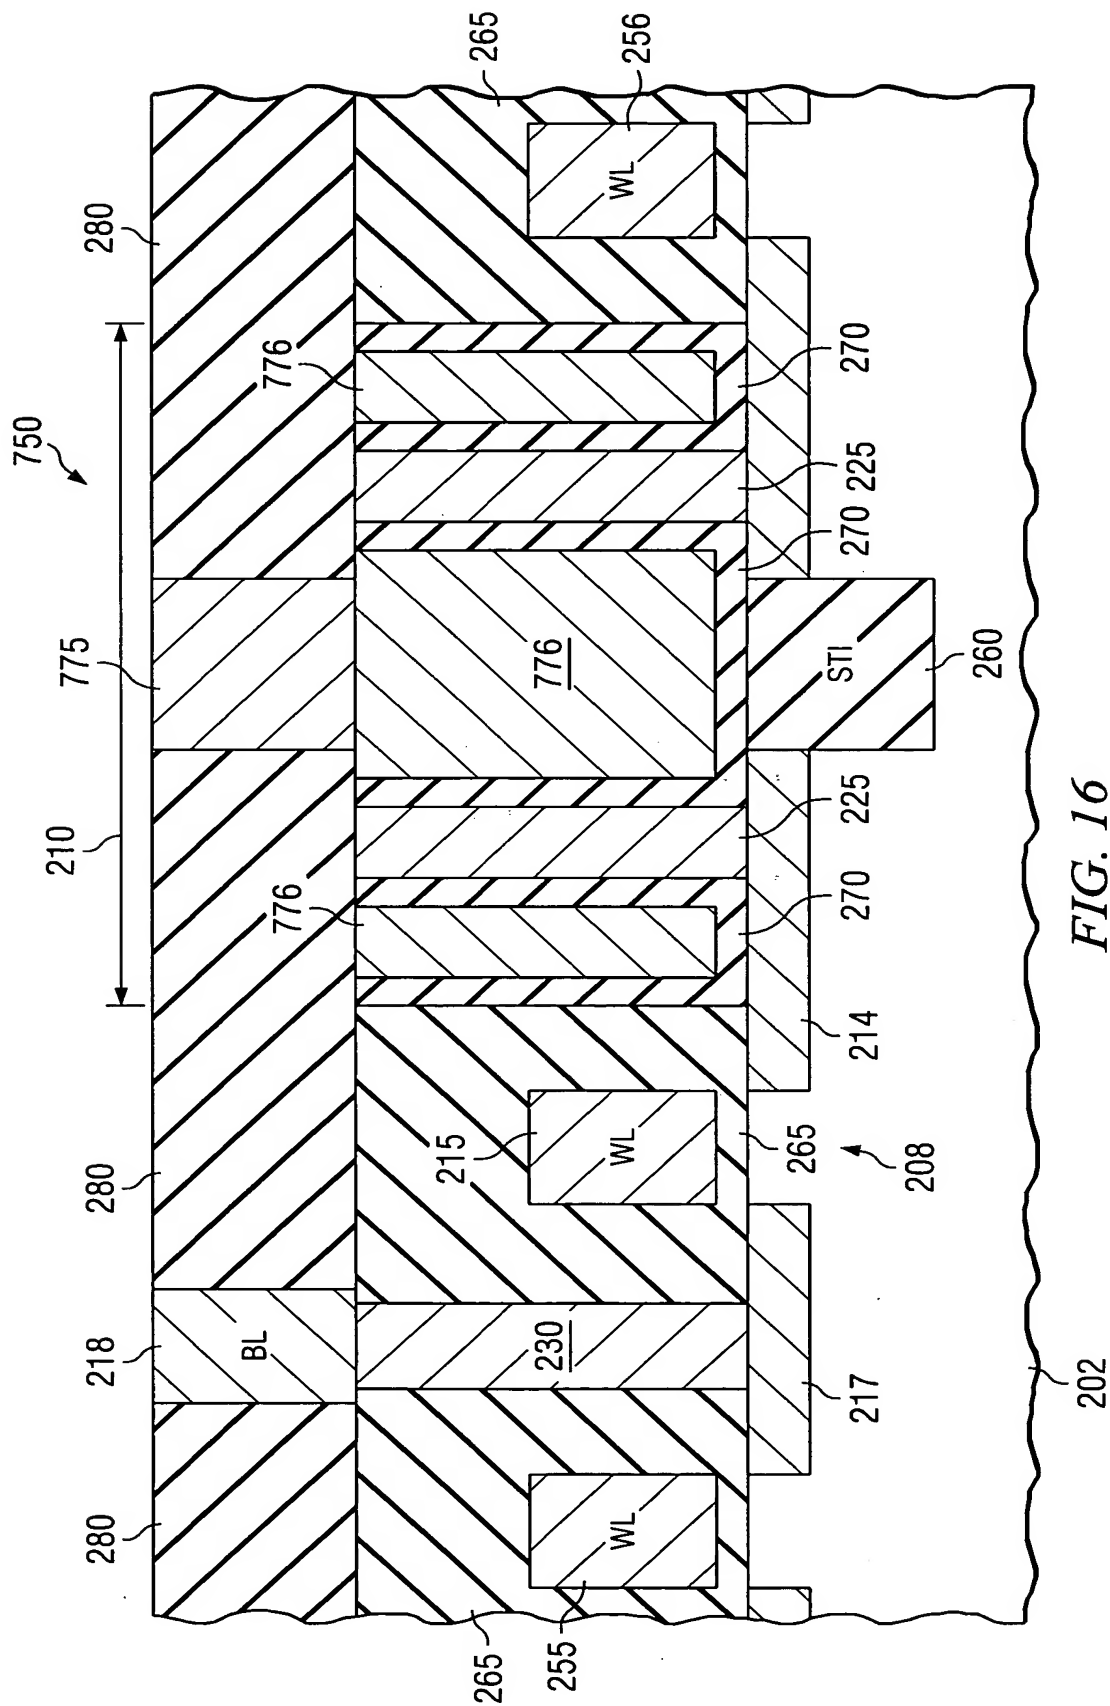


FIG. 16



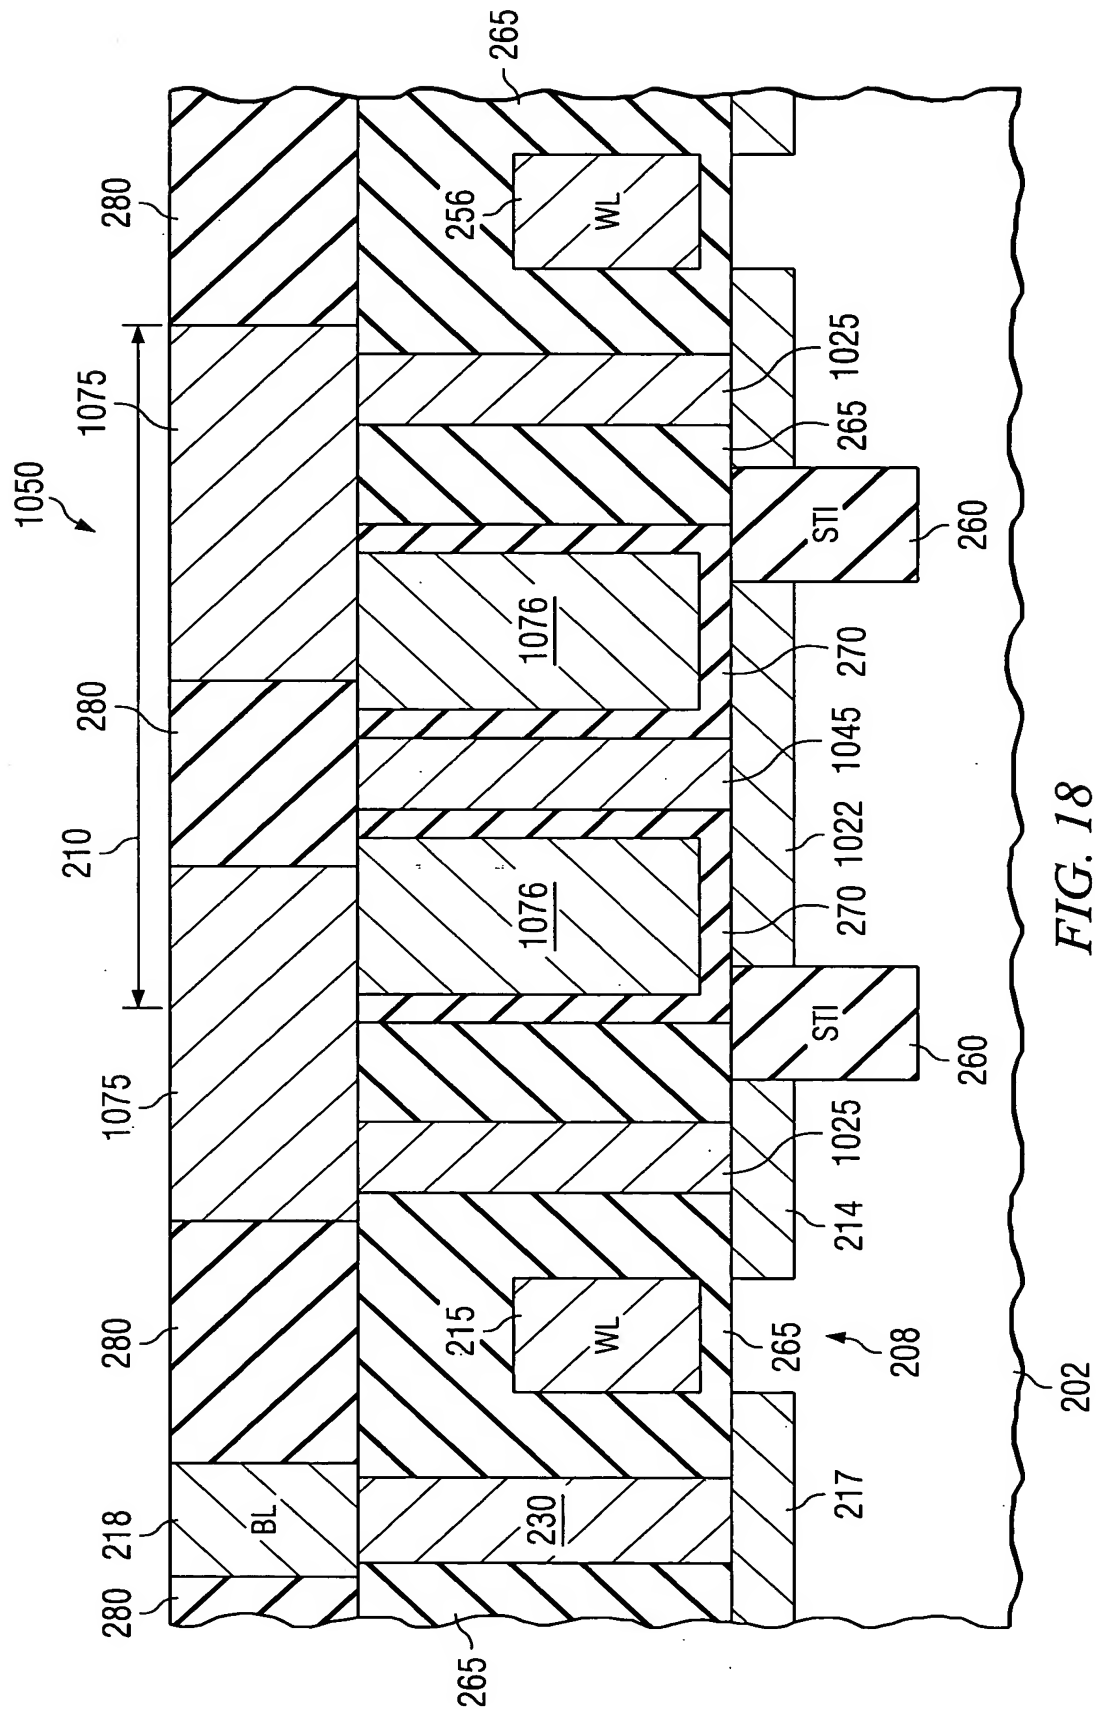

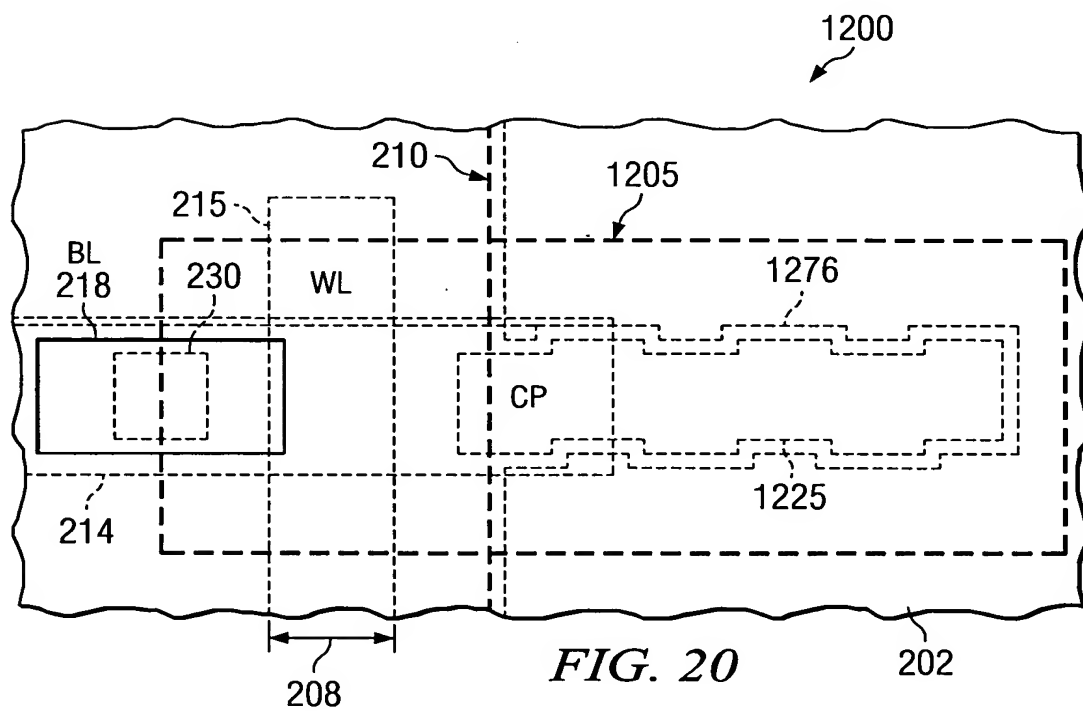

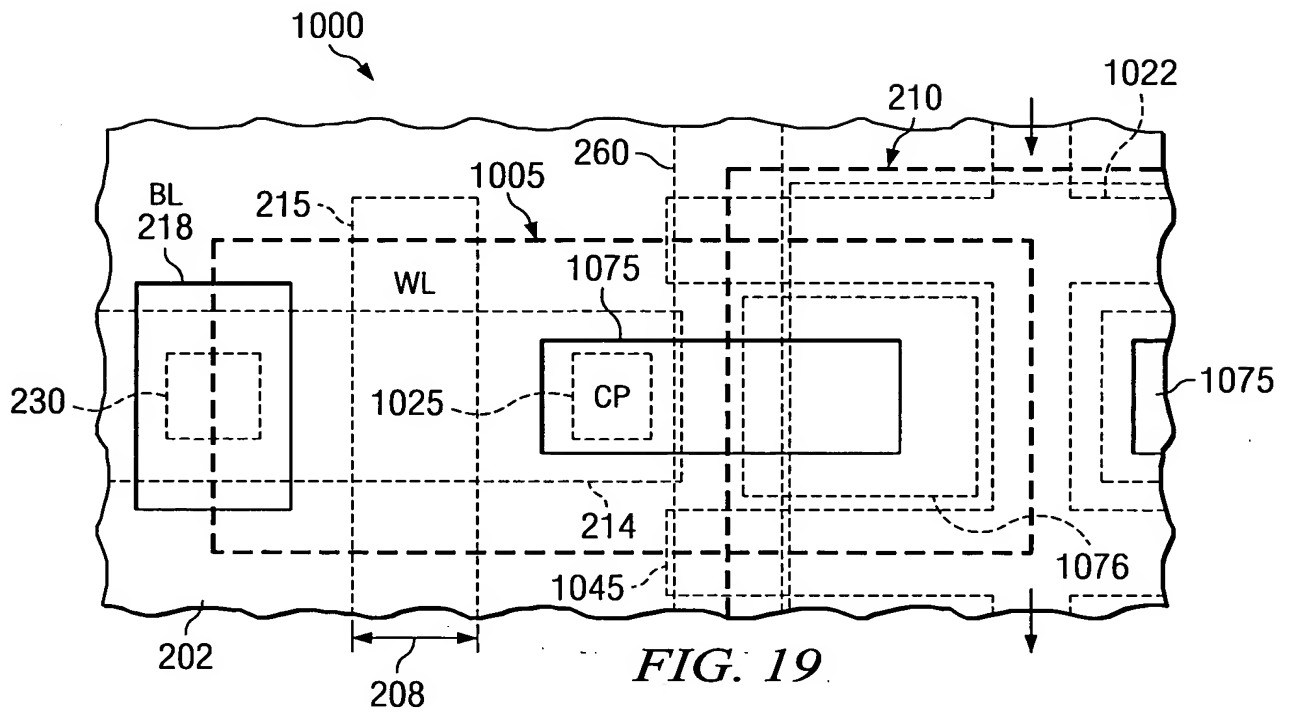

19/26

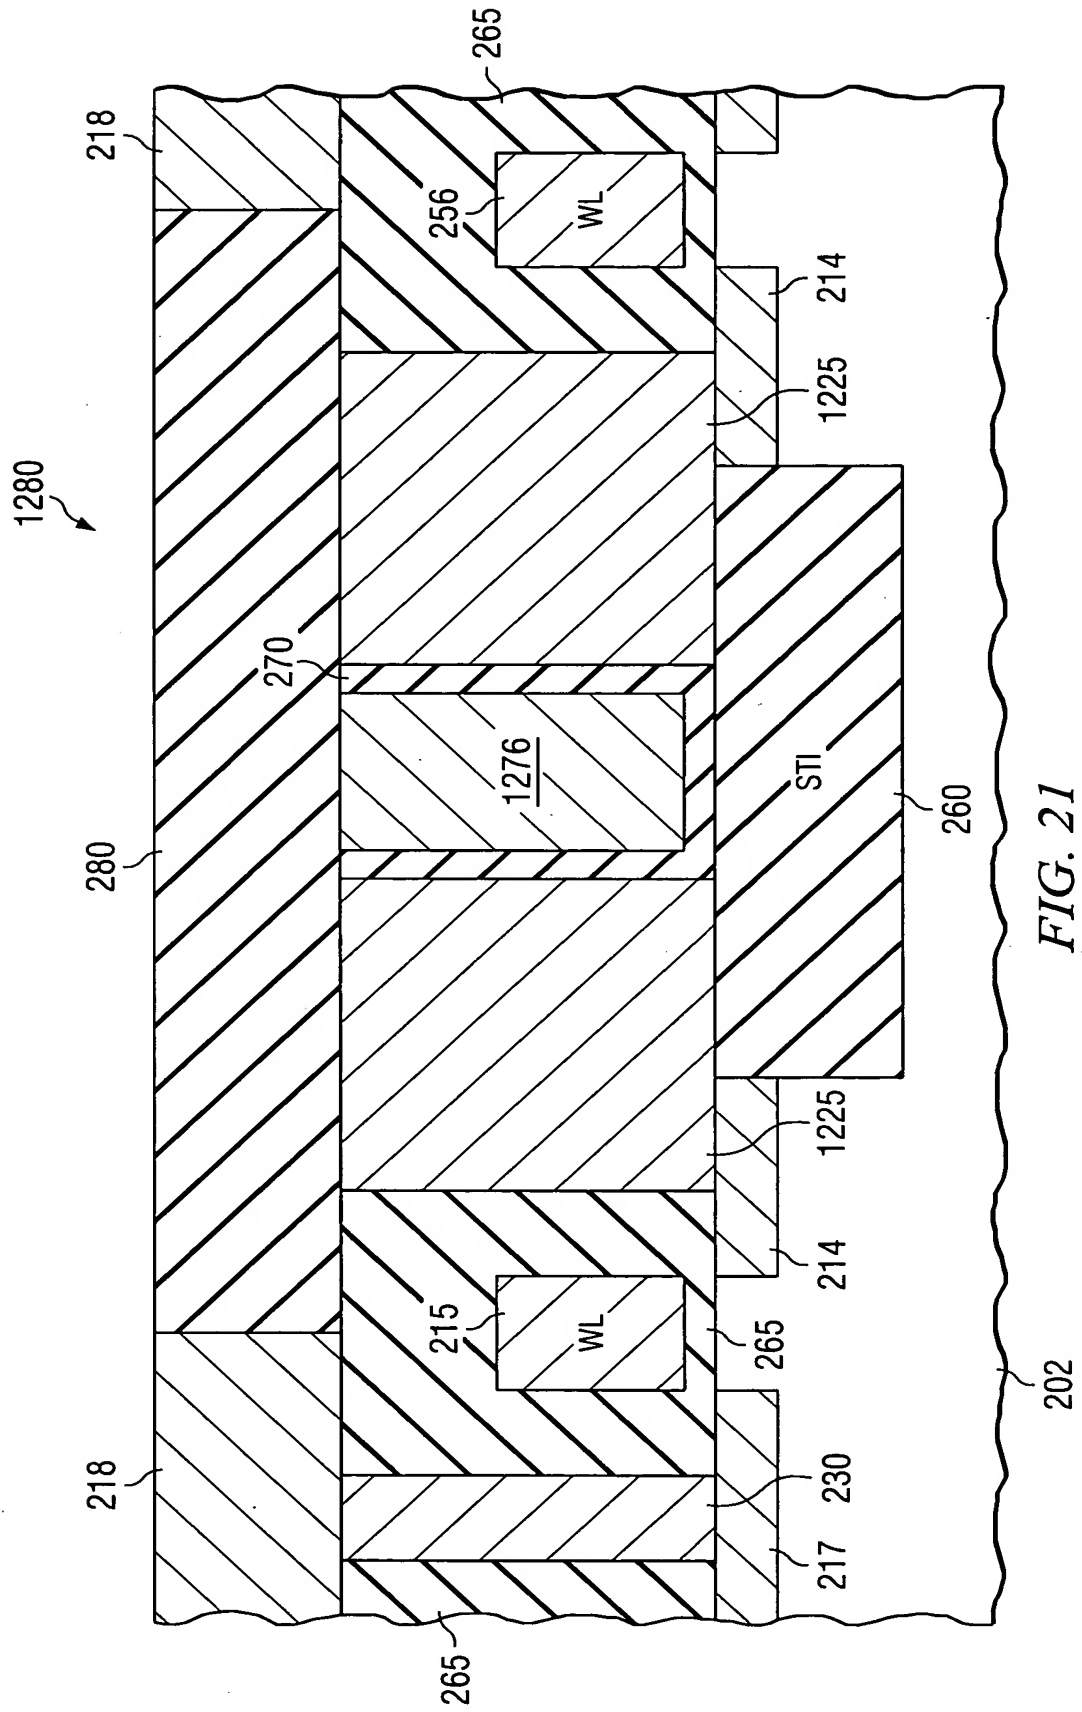
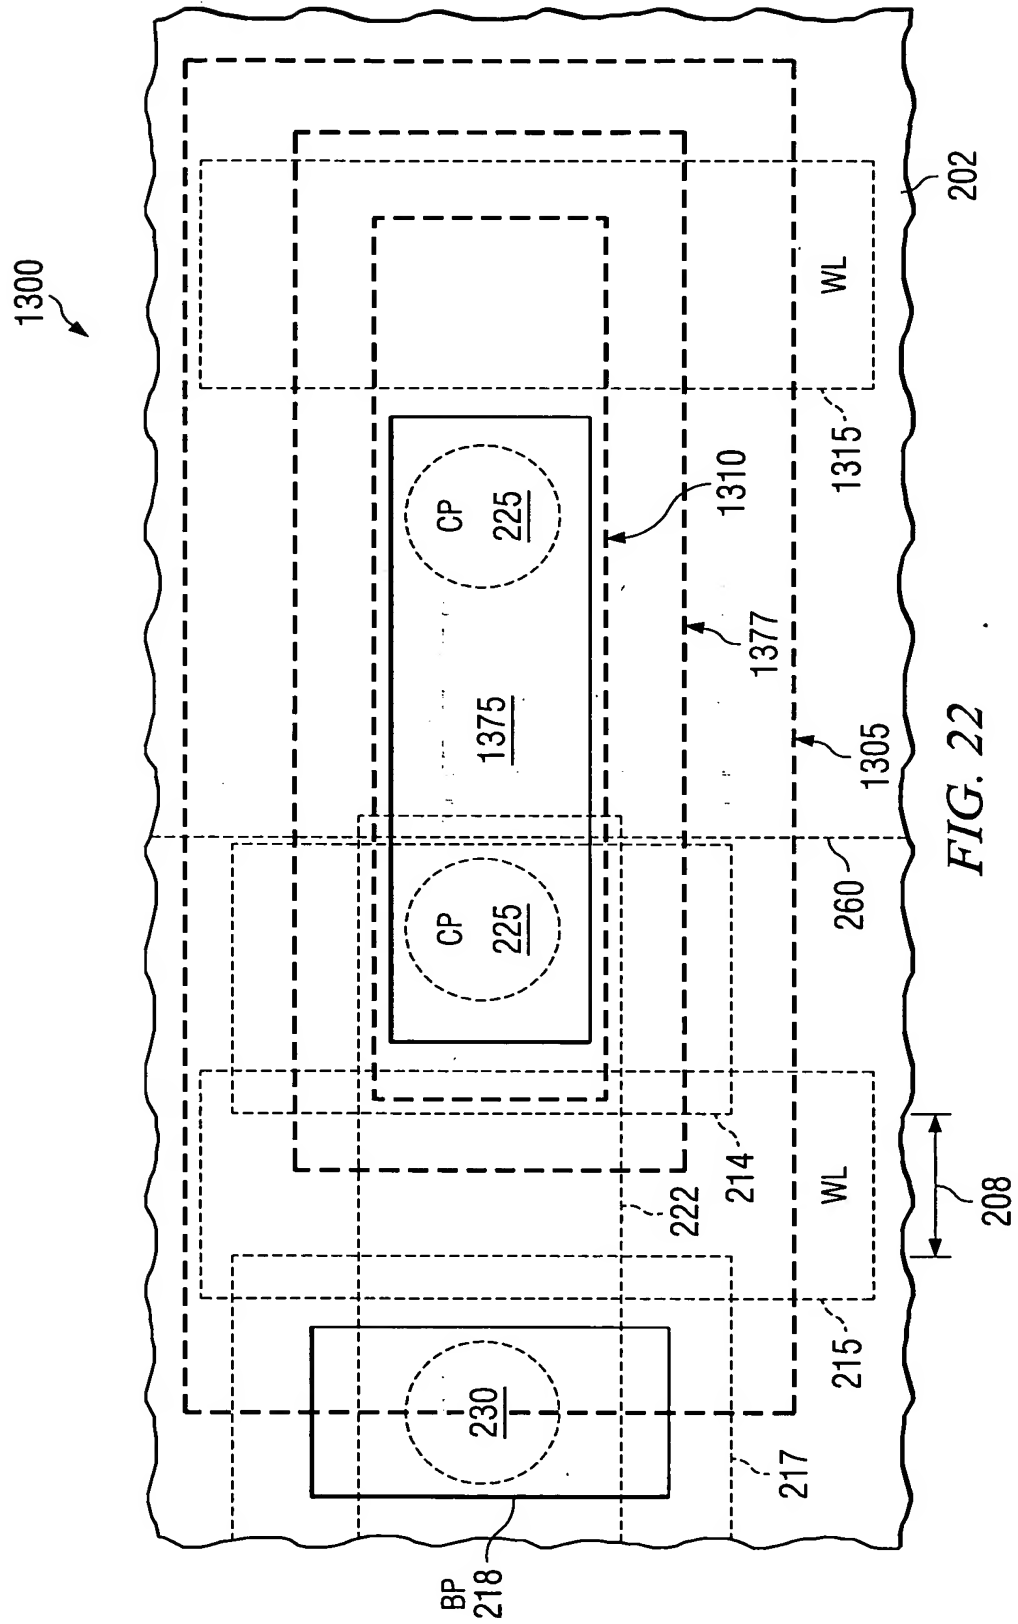


FIG. 21



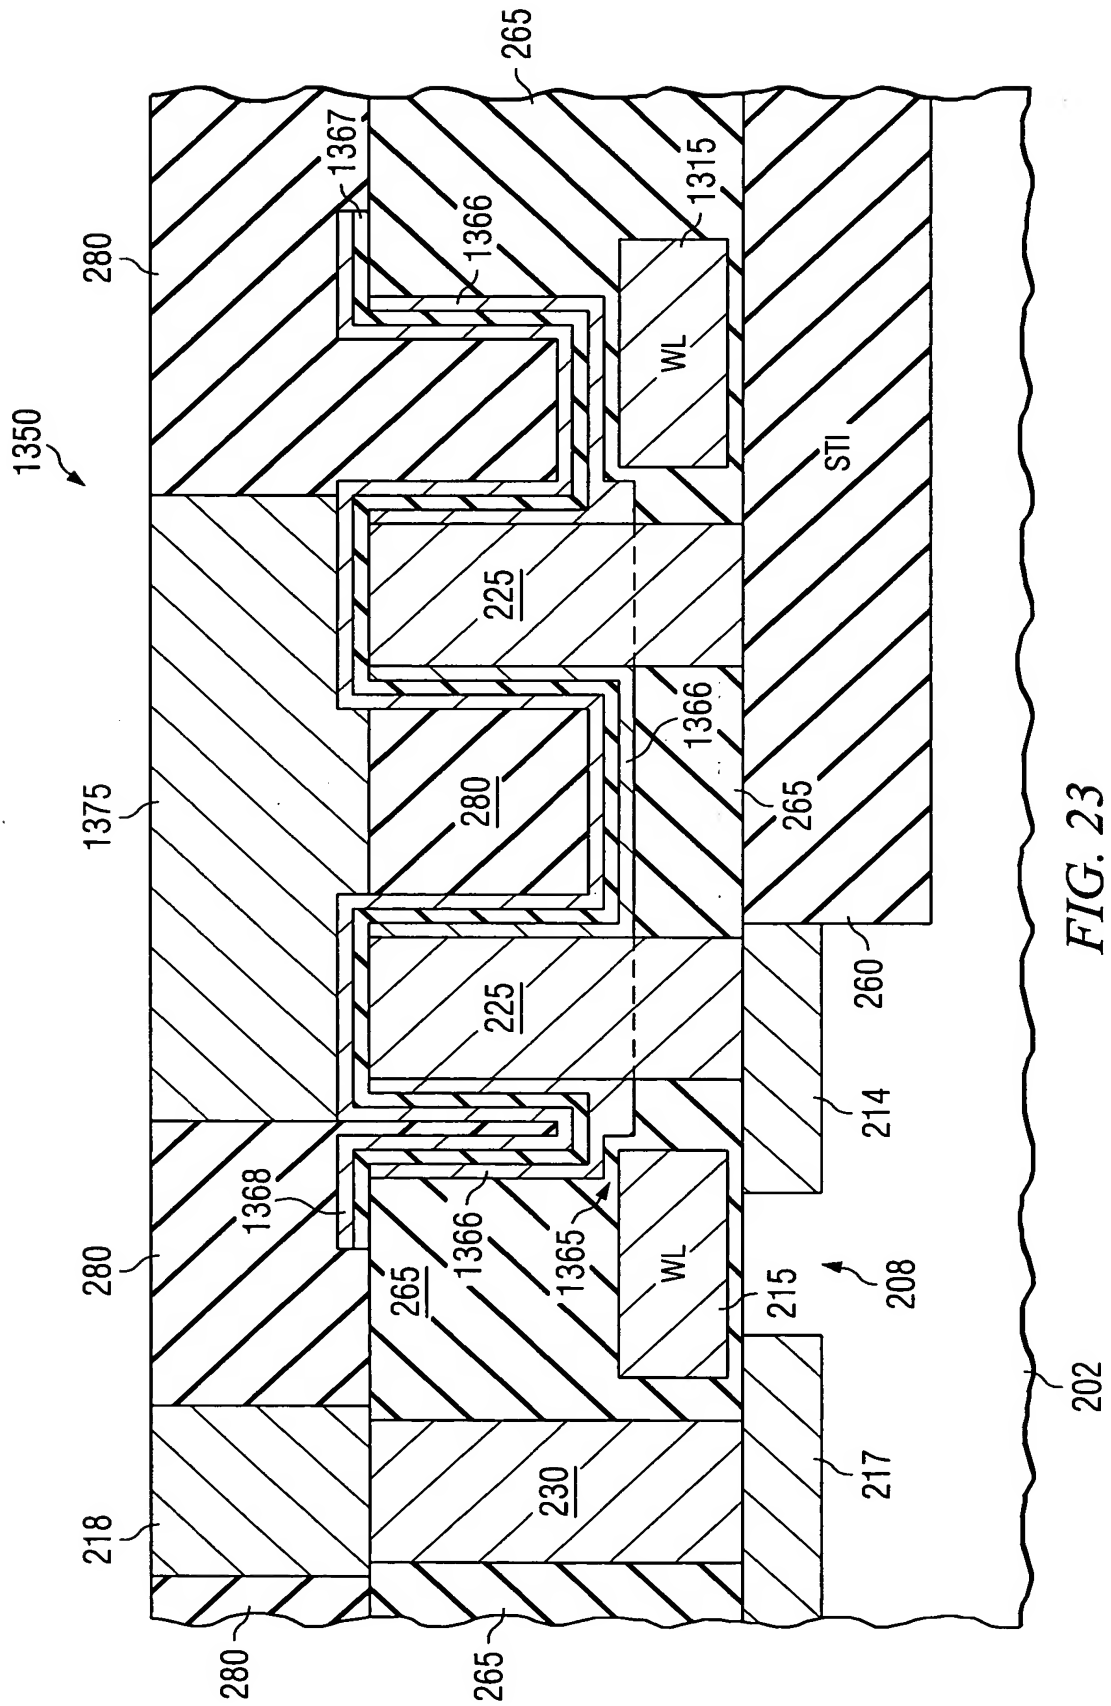


FIG. 23

22/26

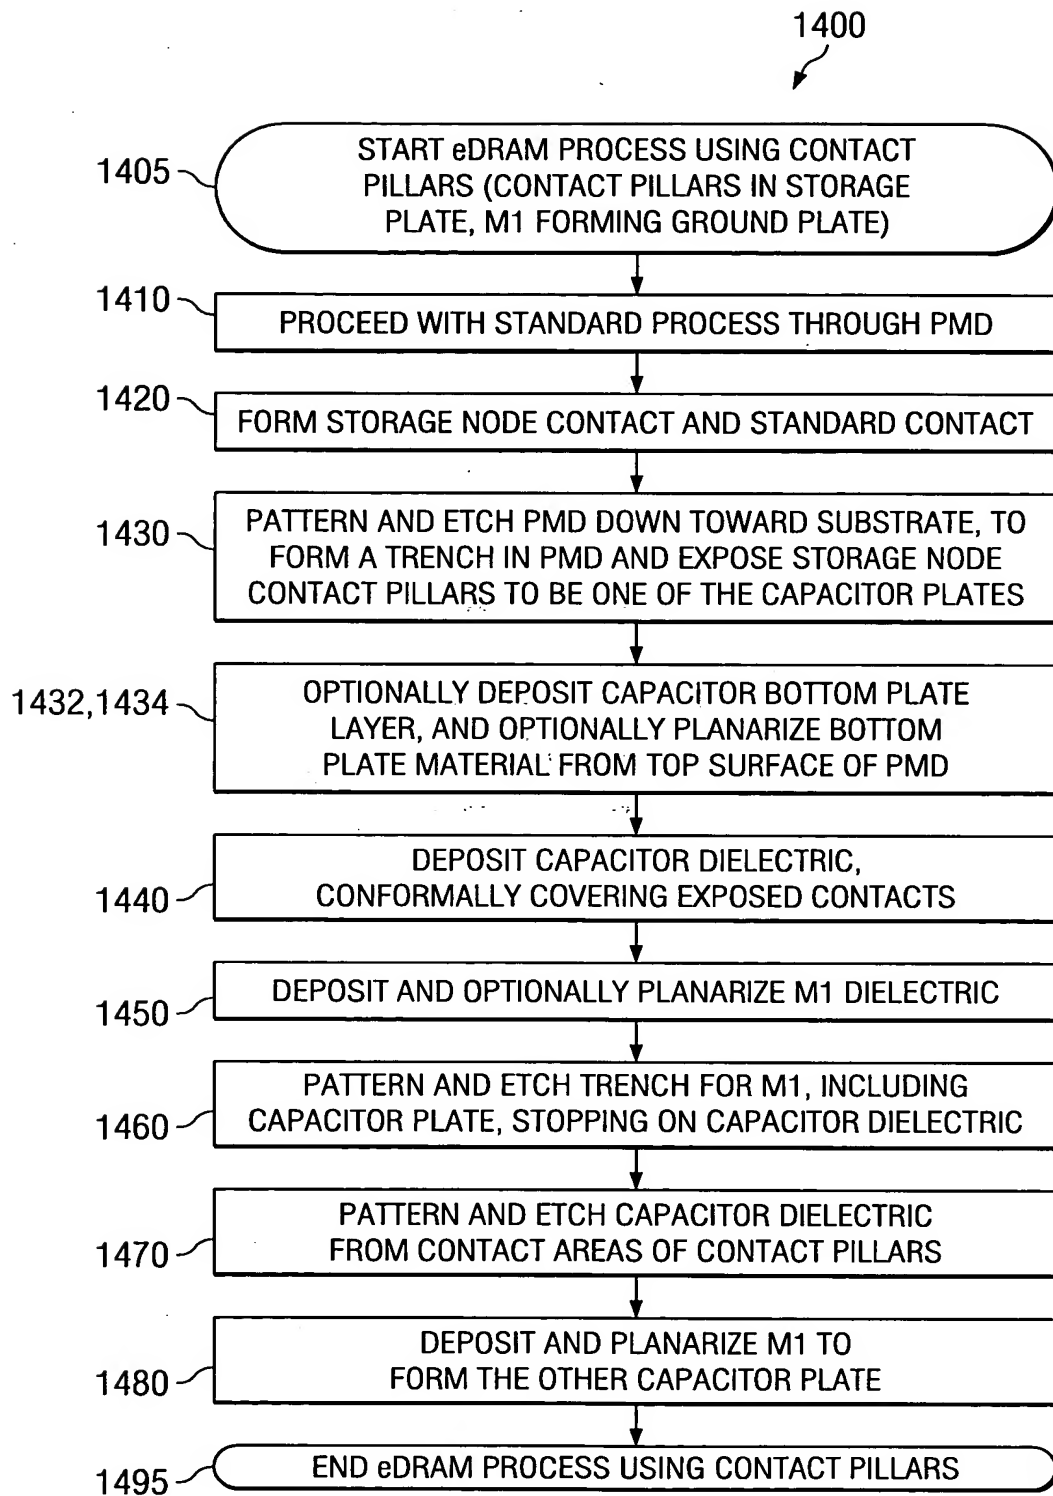


FIG. 24

23/26

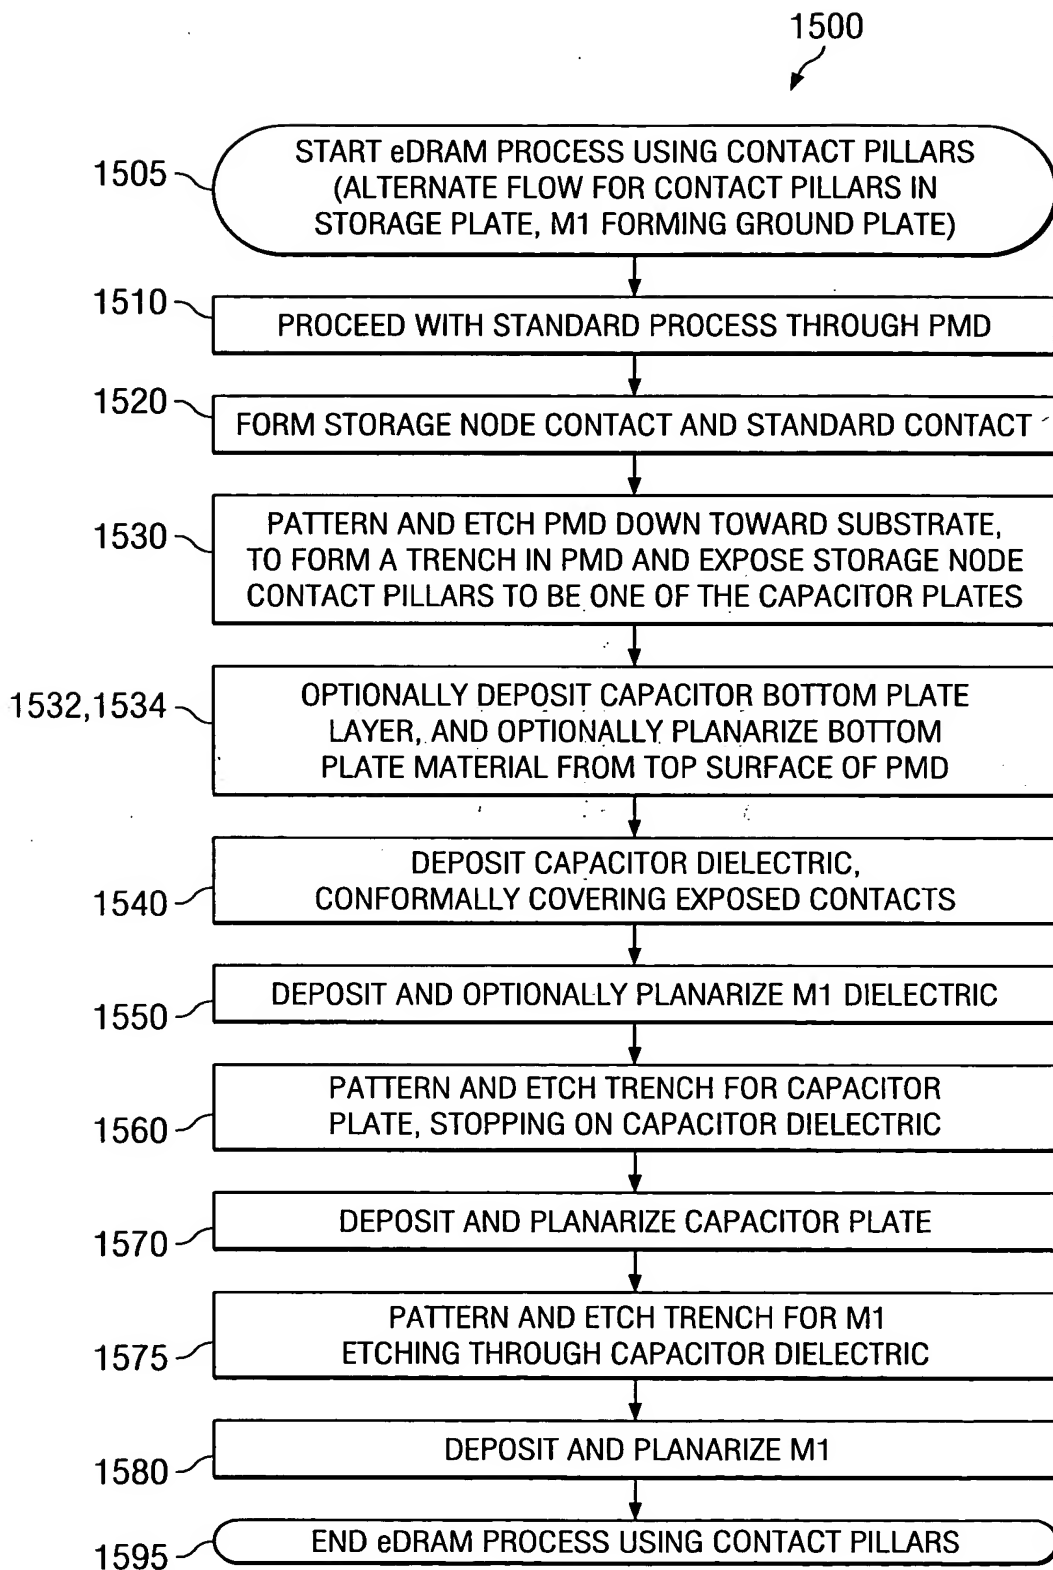


FIG. 25

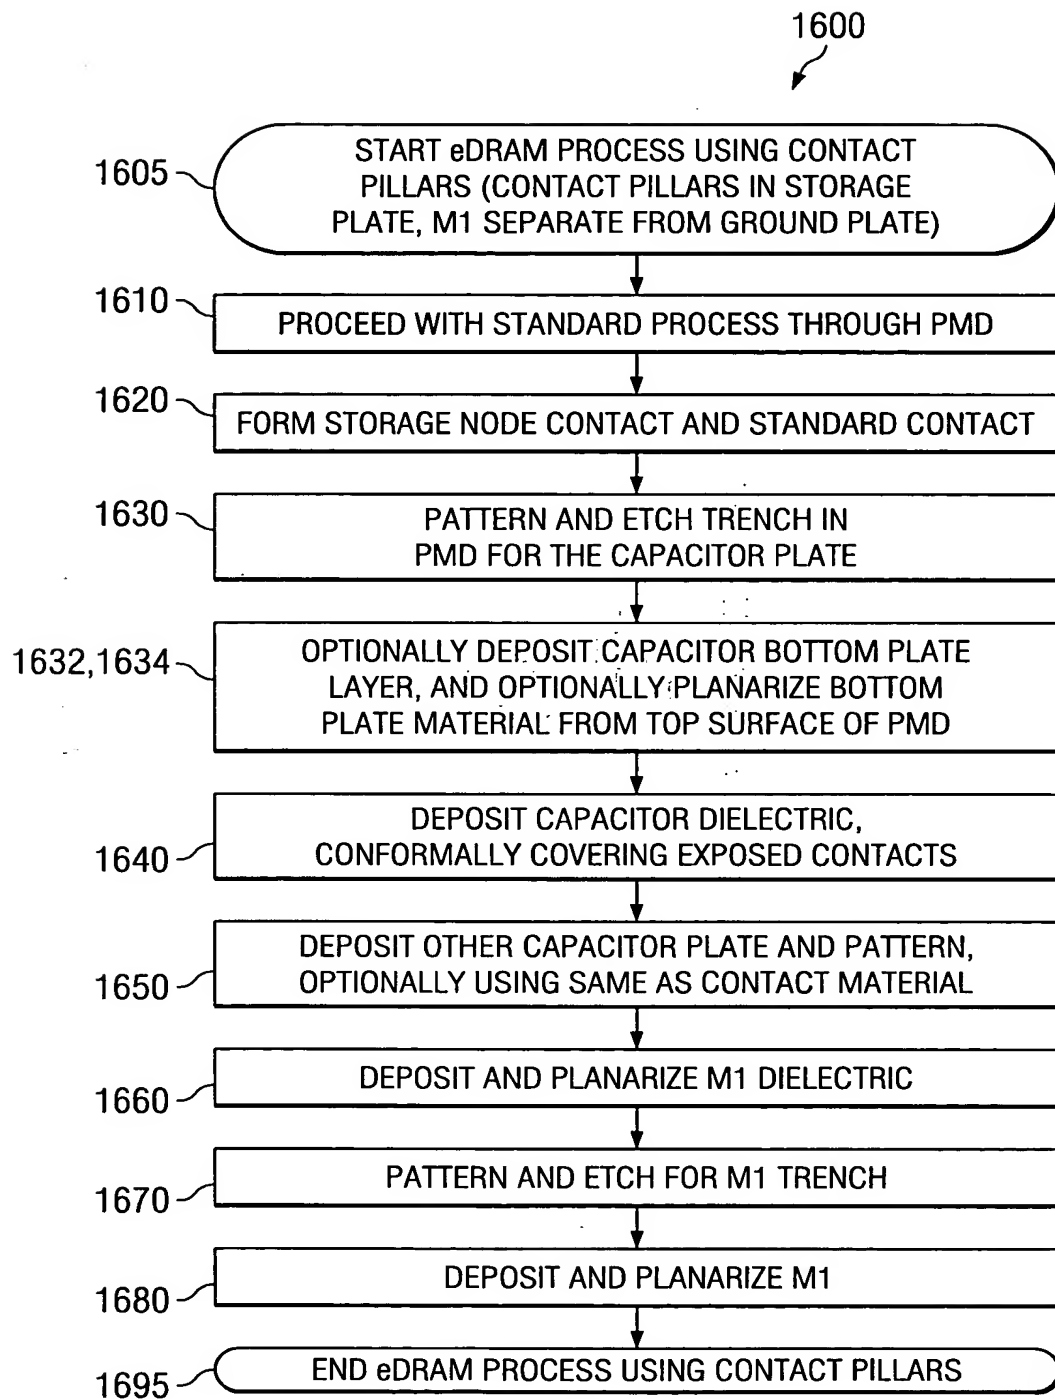


FIG. 26



25/26

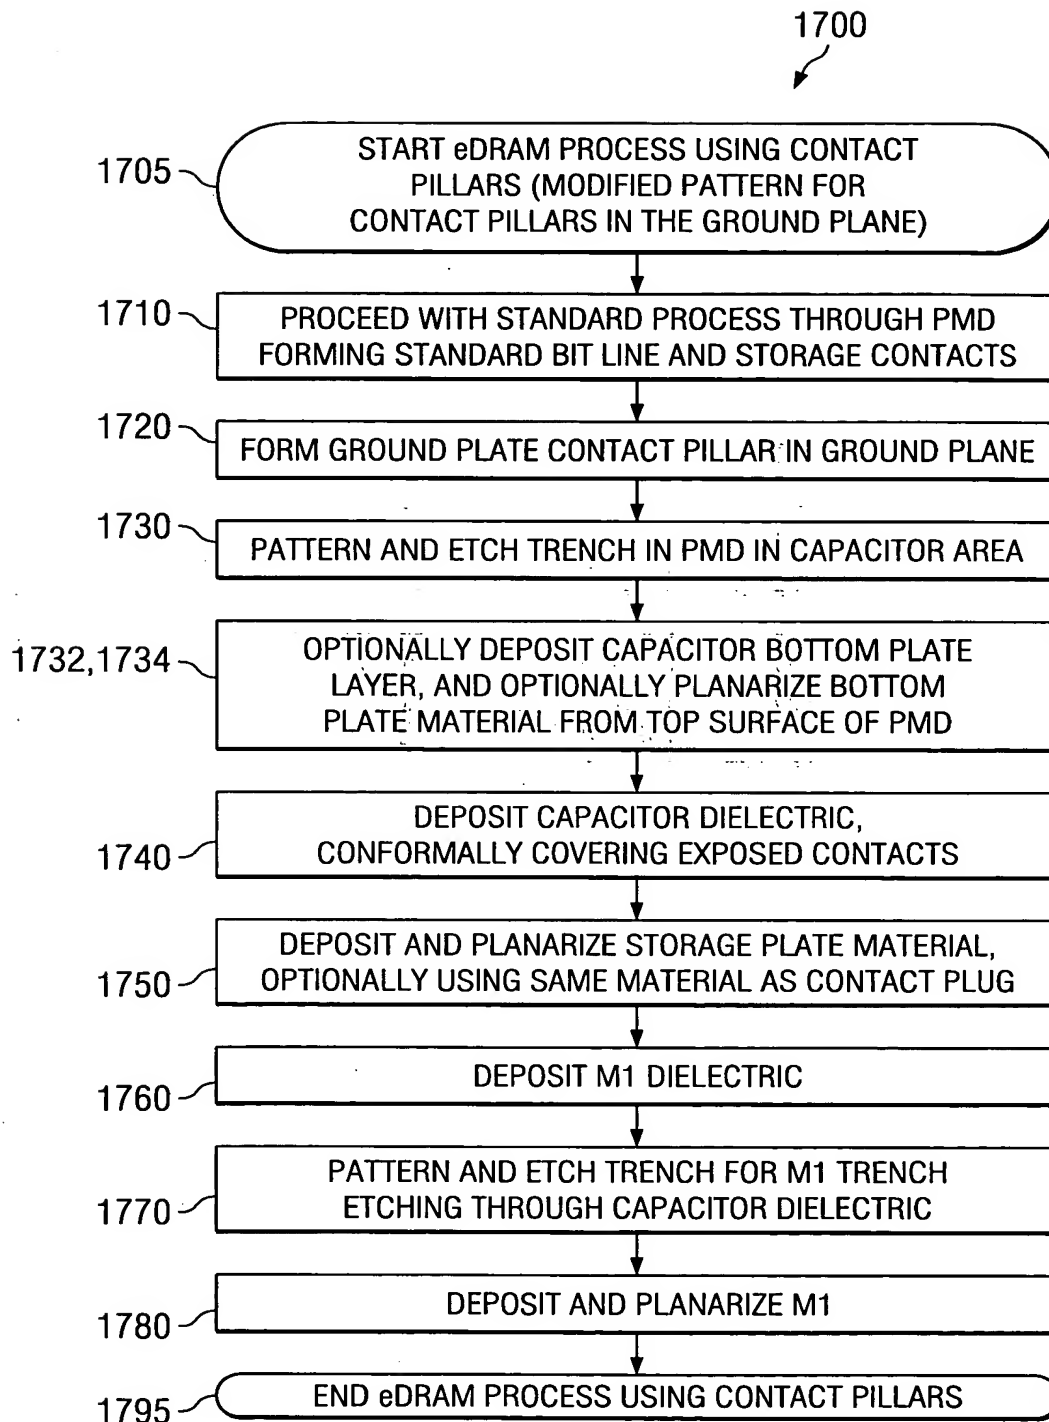


FIG. 27

26/26

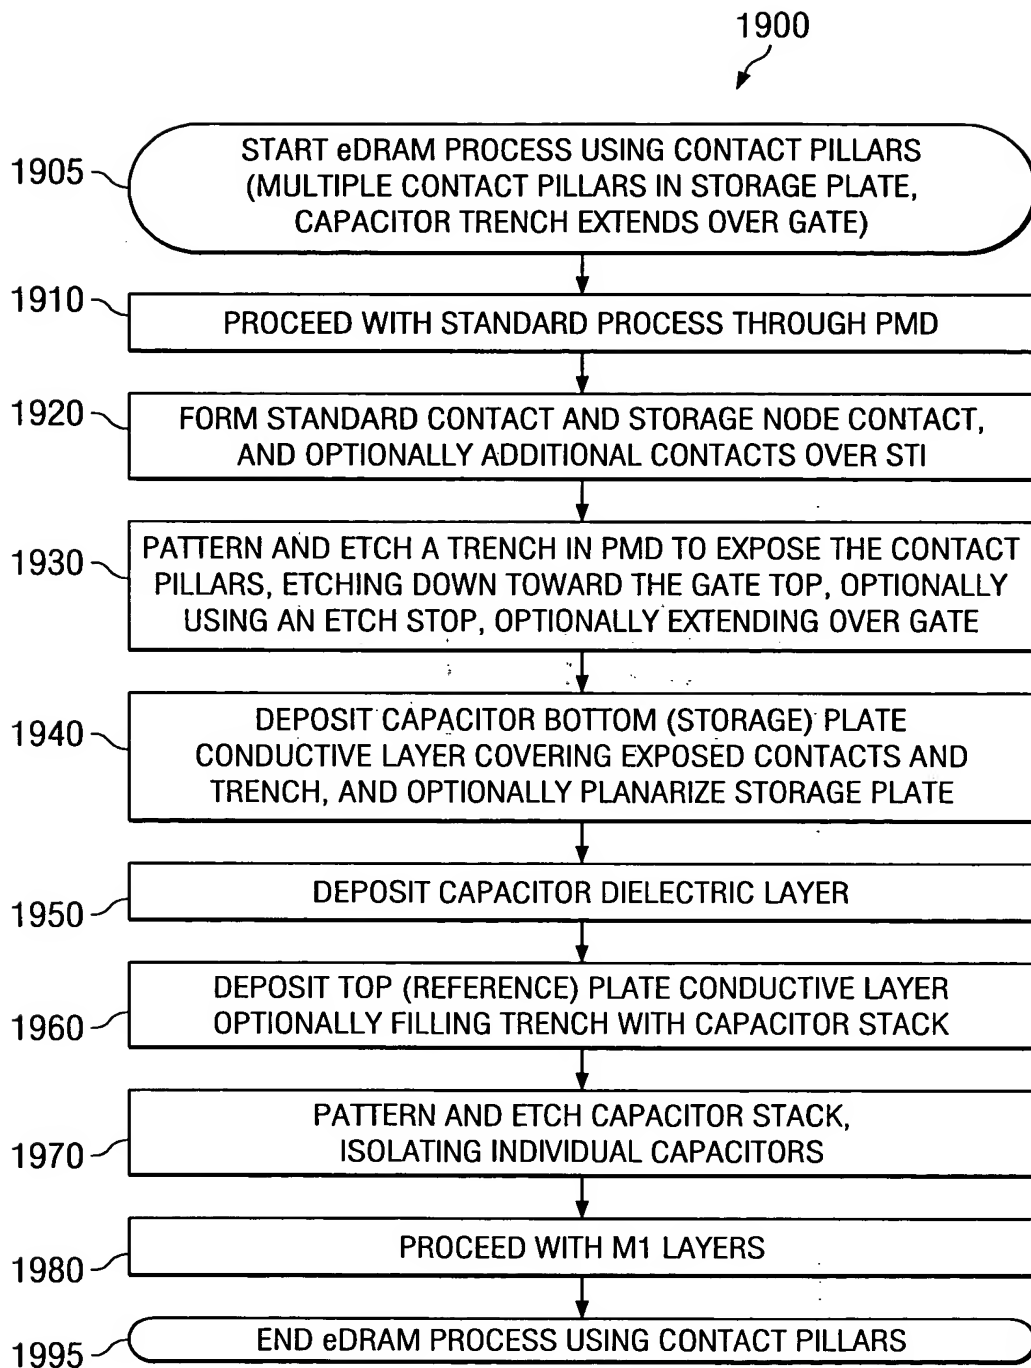


FIG. 28